

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061820\
 Data File : FF007062.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2020 16:46
 Operator : DD\AJ
 Sample : L3031-01 2X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 LOT-11

Integration File: autoint1.e
 Quant Time: Jun 19 01:58:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
 Quant Title :
 QLast Update : Tue Jun 16 04:06:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1432698	12.170 ug/ml
Target Compounds			
4) N-TETRADECANE	8.339f	159806	1.169 ug/ml
7) N-EICOSANE	12.698f	1773609	12.984 ug/ml
10) N-TETRACOSANE	14.917	921987	5.607 ug/ml
12) N-OCTACOSANE	16.915	286641	1.923 ug/ml
13) N-TRIACONTANE	17.802	302198	2.014 ug/ml
14) N-DOTRIACONTANE	18.630	228547	1.654 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061820\
Data File : FF007062.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2020 16:46
Operator : DD\AJ
Sample : L3031-01 2X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
LOT-11

Integration File: autoint1.e
Quant Time: Jun 19 01:58:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

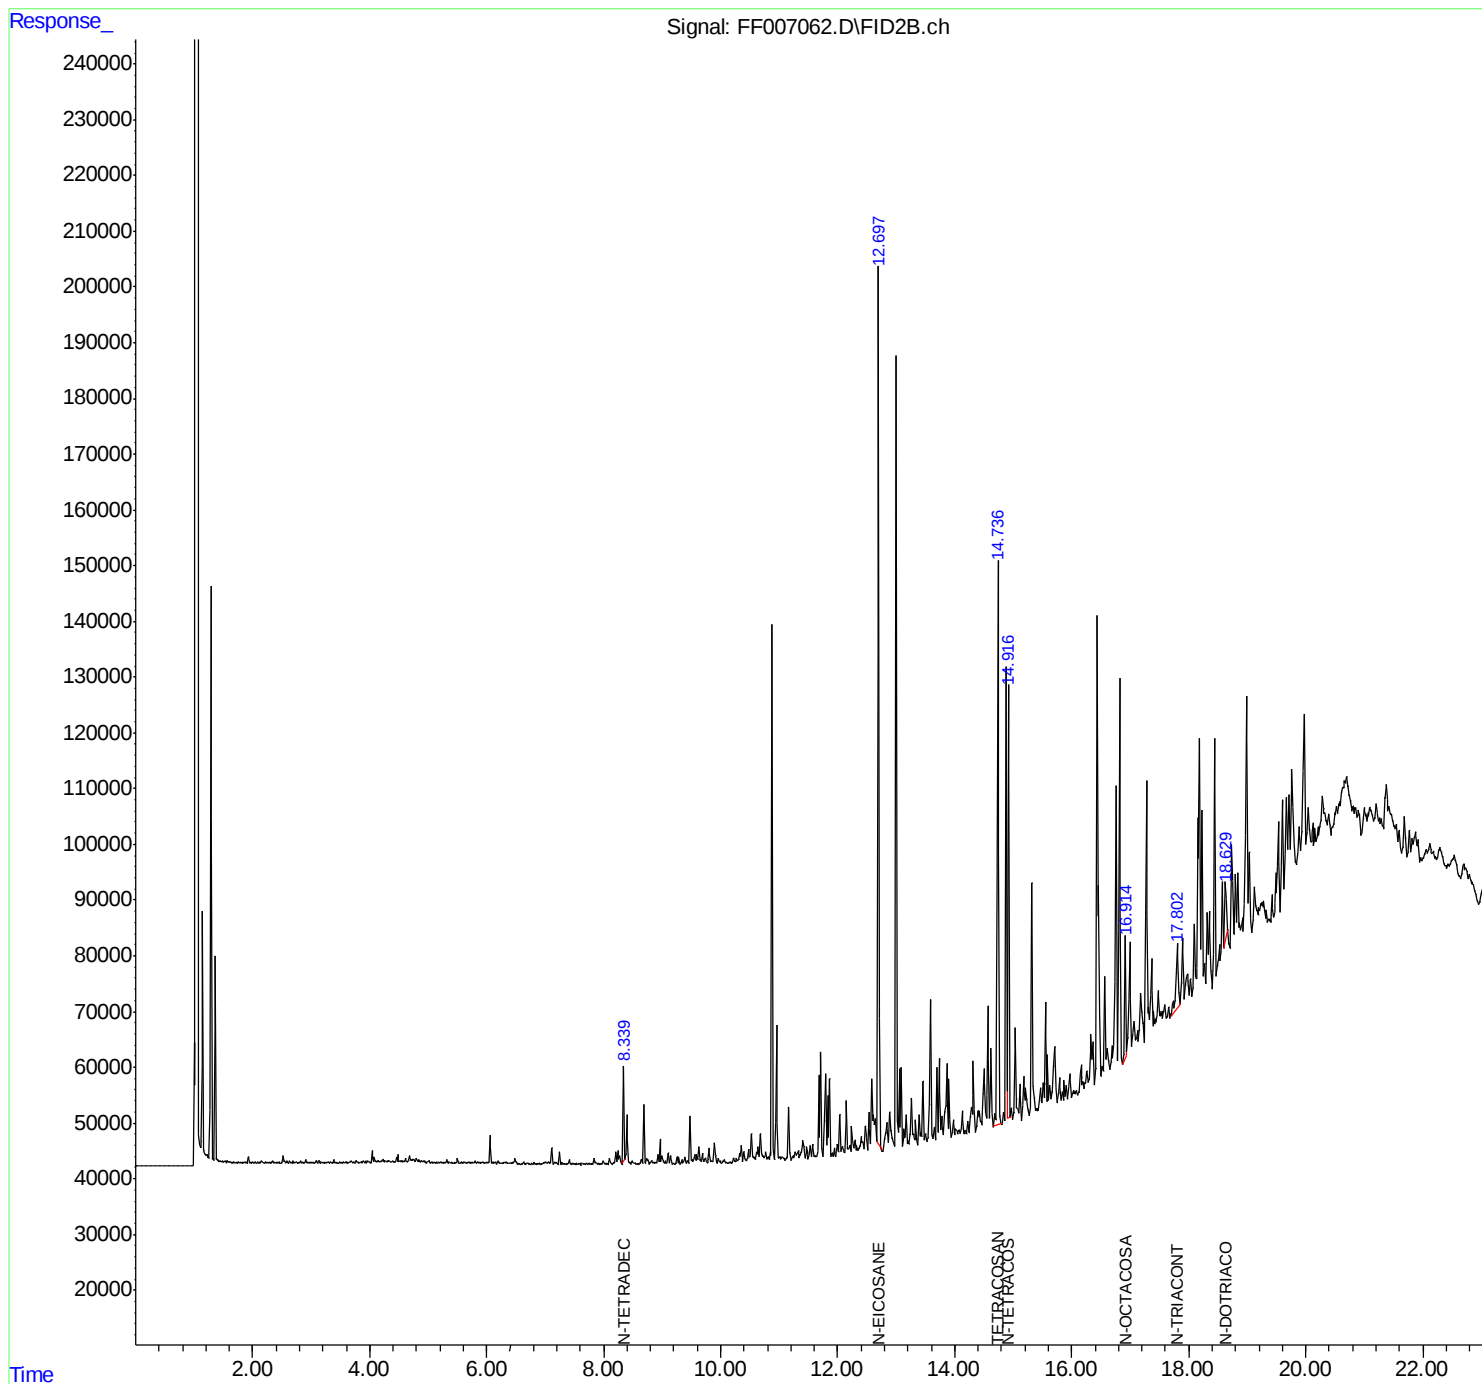


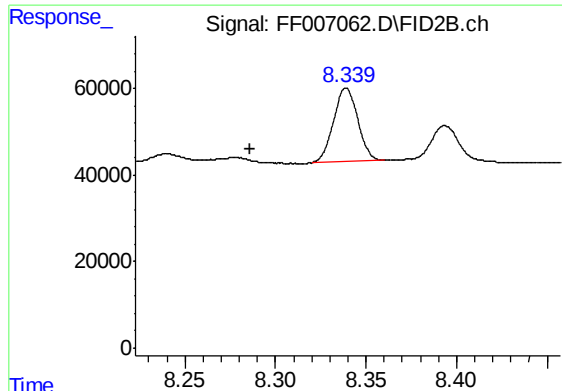

#4 N-TETRADECANE


R.T.: 8.339 min
Delta R.T.: 0.053 min
Response: 159806
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :
LOT-11

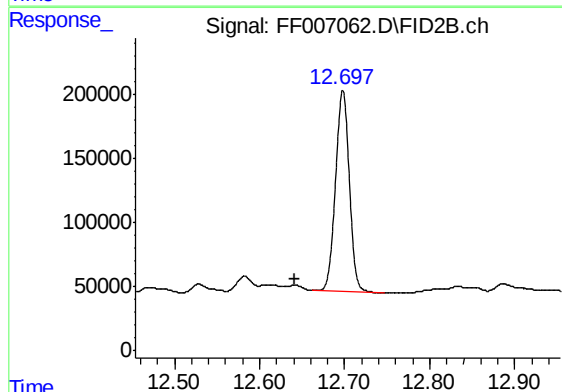


#7 N-EICOSANE

R.T.: 12.698 min
Delta R.T.: 0.057 min
Response: 1773609
Conc: 12.98 ug/ml

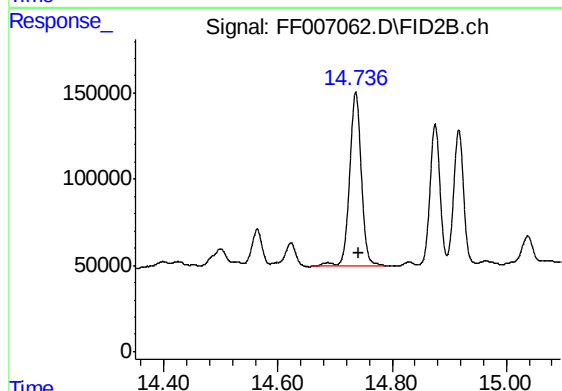


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.004 min
Response: 1432698
Conc: 12.17 ug/ml

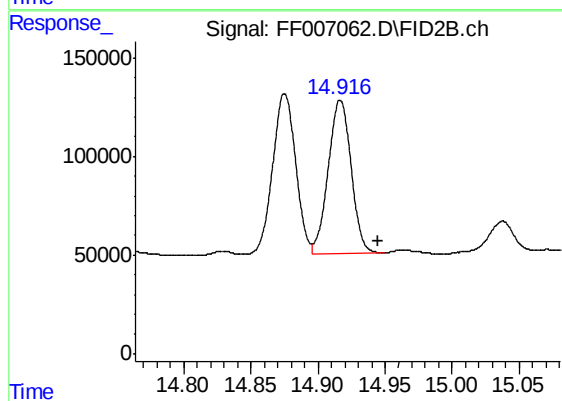

#10 N-TETRACOSANE


R.T.: 14.917 min
Delta R.T.: -0.028 min
Response: 921987
Conc: 5.61 ug/ml

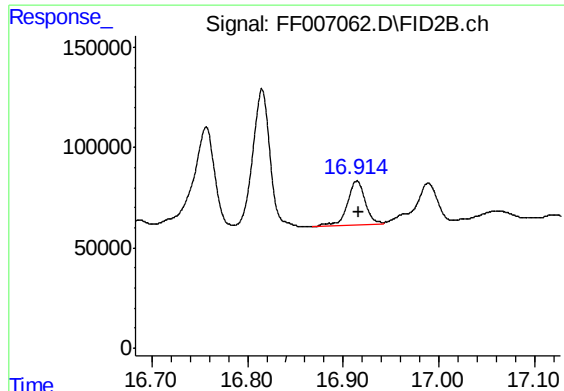

#12 N-OCTACOSANE


R.T.: 16.915 min
Delta R.T.: -0.002 min
Response: 286641
Conc: 1.92 ug/ml

Instrument :
FID_F
ClientSampleId :
LOT-11

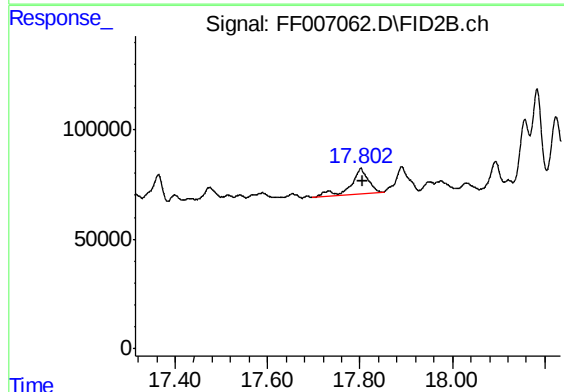

#13 N-TRIACONTANE

R.T.: 17.802 min
Delta R.T.: -0.003 min
Response: 302198
Conc: 2.01 ug/ml

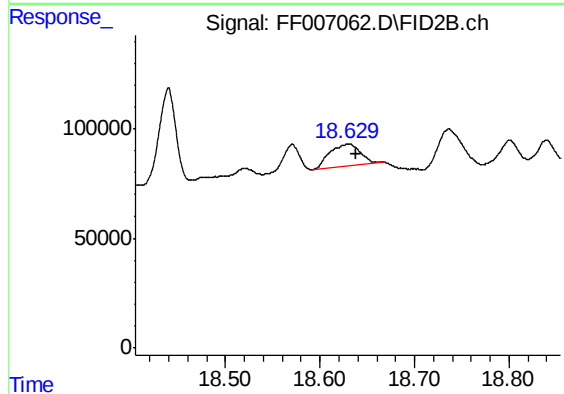

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: -0.008 min
Response: 228547
Conc: 1.65 ug/ml