

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF061820\  
 Data File : FF007063.D  
 Signal(s) : FID2B.ch  
 Acq On : 18 Jun 2020 17:17  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 I.BLK

Integration File: autoint1.e  
 Quant Time: Jun 19 01:58:23 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF061520.M  
 Quant Title :  
 QLast Update : Tue Jun 16 04:06:59 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	2299178	19.531 ug/ml
Target Compounds			
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF061820\  
 Data File : FF007063.D  
 Signal(s) : FID2B.ch  
 Acq On : 18 Jun 2020 17:17  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 I.BLK

Integration File: autoint1.e  
 Quant Time: Jun 19 01:58:23 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF061520.M  
 Quant Title :  
 QLast Update : Tue Jun 16 04:06:59 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

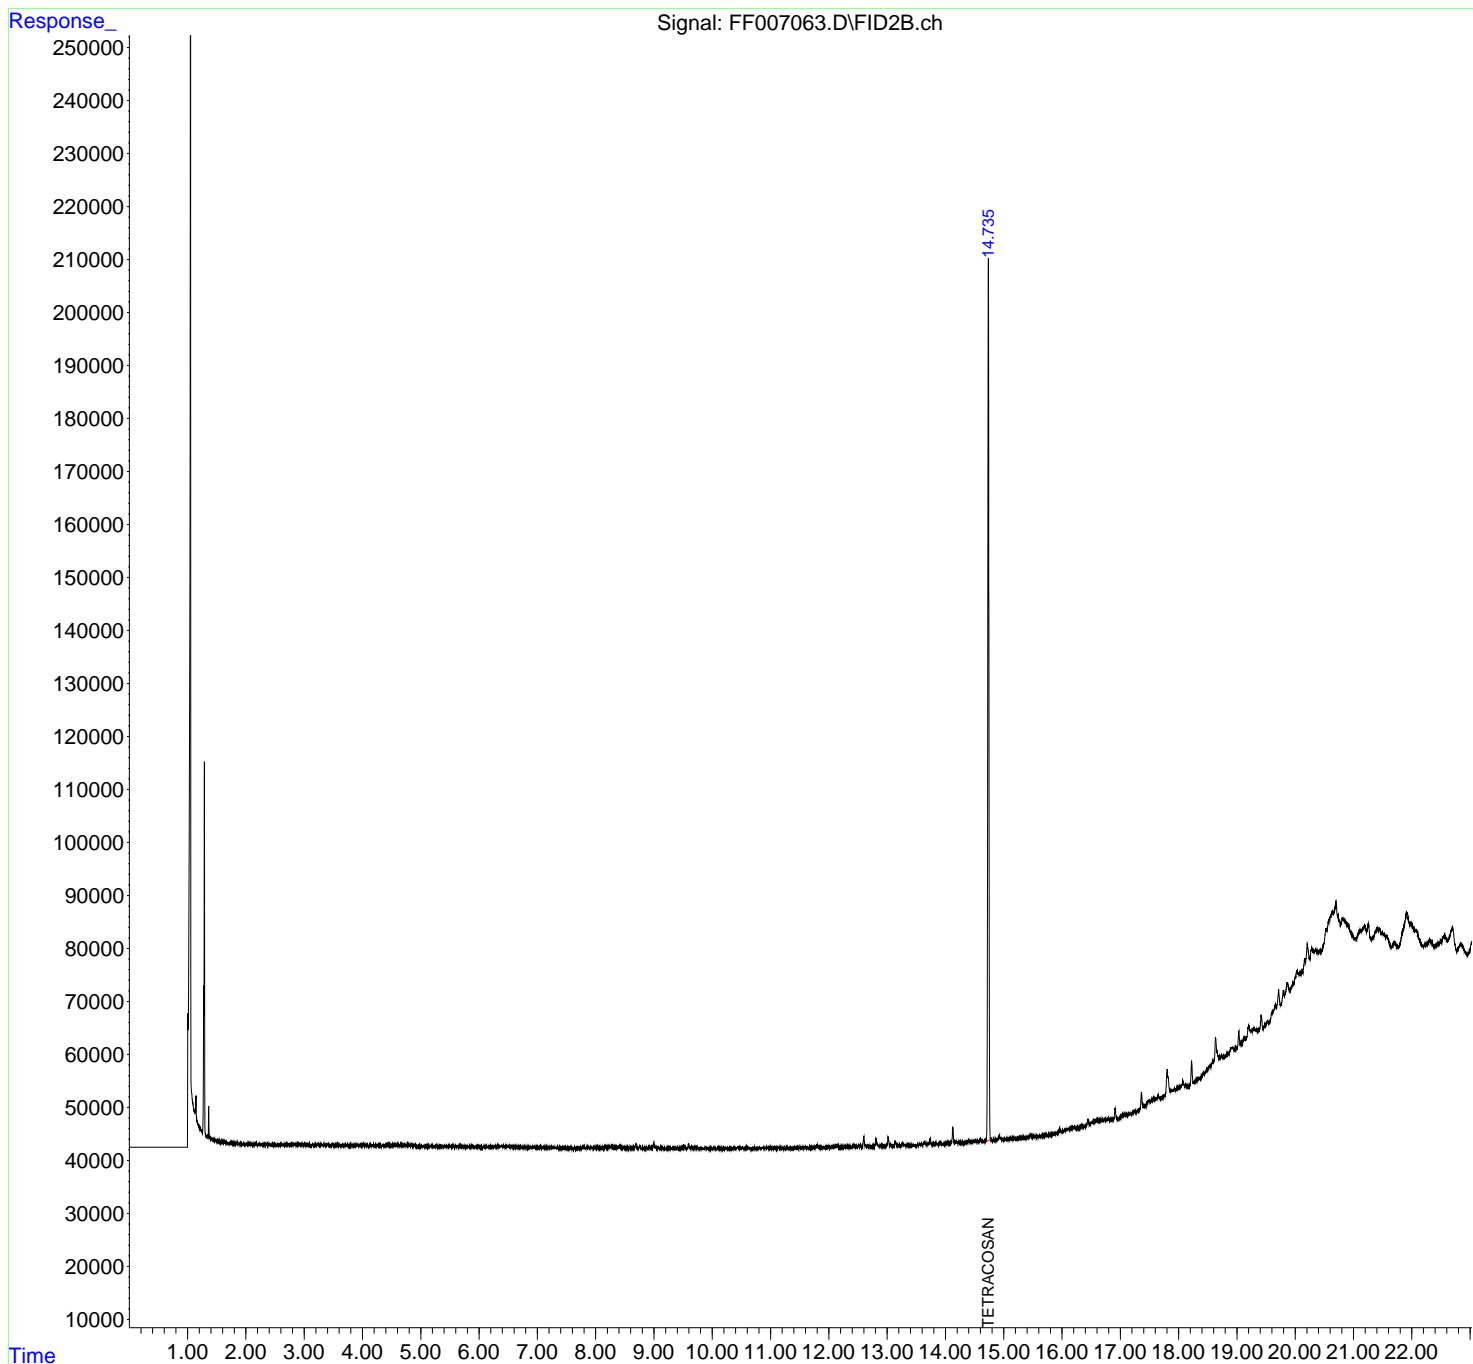

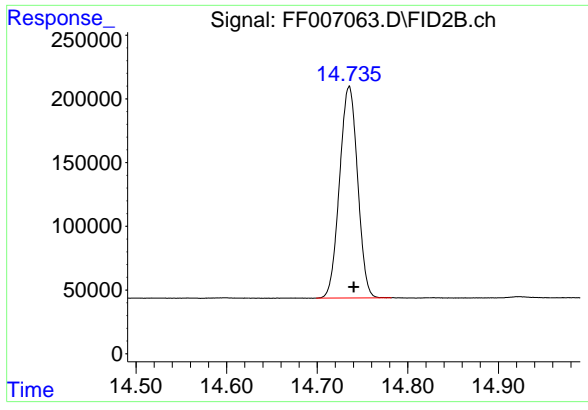

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min  
Delta R.T.: -0.005 min  
Response: 2299178  
Conc: 19.53 ug/ml

Instrument :  
FID\_F  
ClientSampled :  
I.BLK