

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061920\
Data File : FF007076.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2020 17:51
Operator : DD\AJ
Sample : L3056-01 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SAMPLE-A-LOT-11

Integration File: Sample.e
Quant Time: Jun 20 00:34:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	372597	3.165 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061920\
Data File : FF007076.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2020 17:51
Operator : DD\AJ
Sample : L3056-01 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SAMPLE-A-LOT-11

Integration File: Sample.e
Quant Time: Jun 20 00:34:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

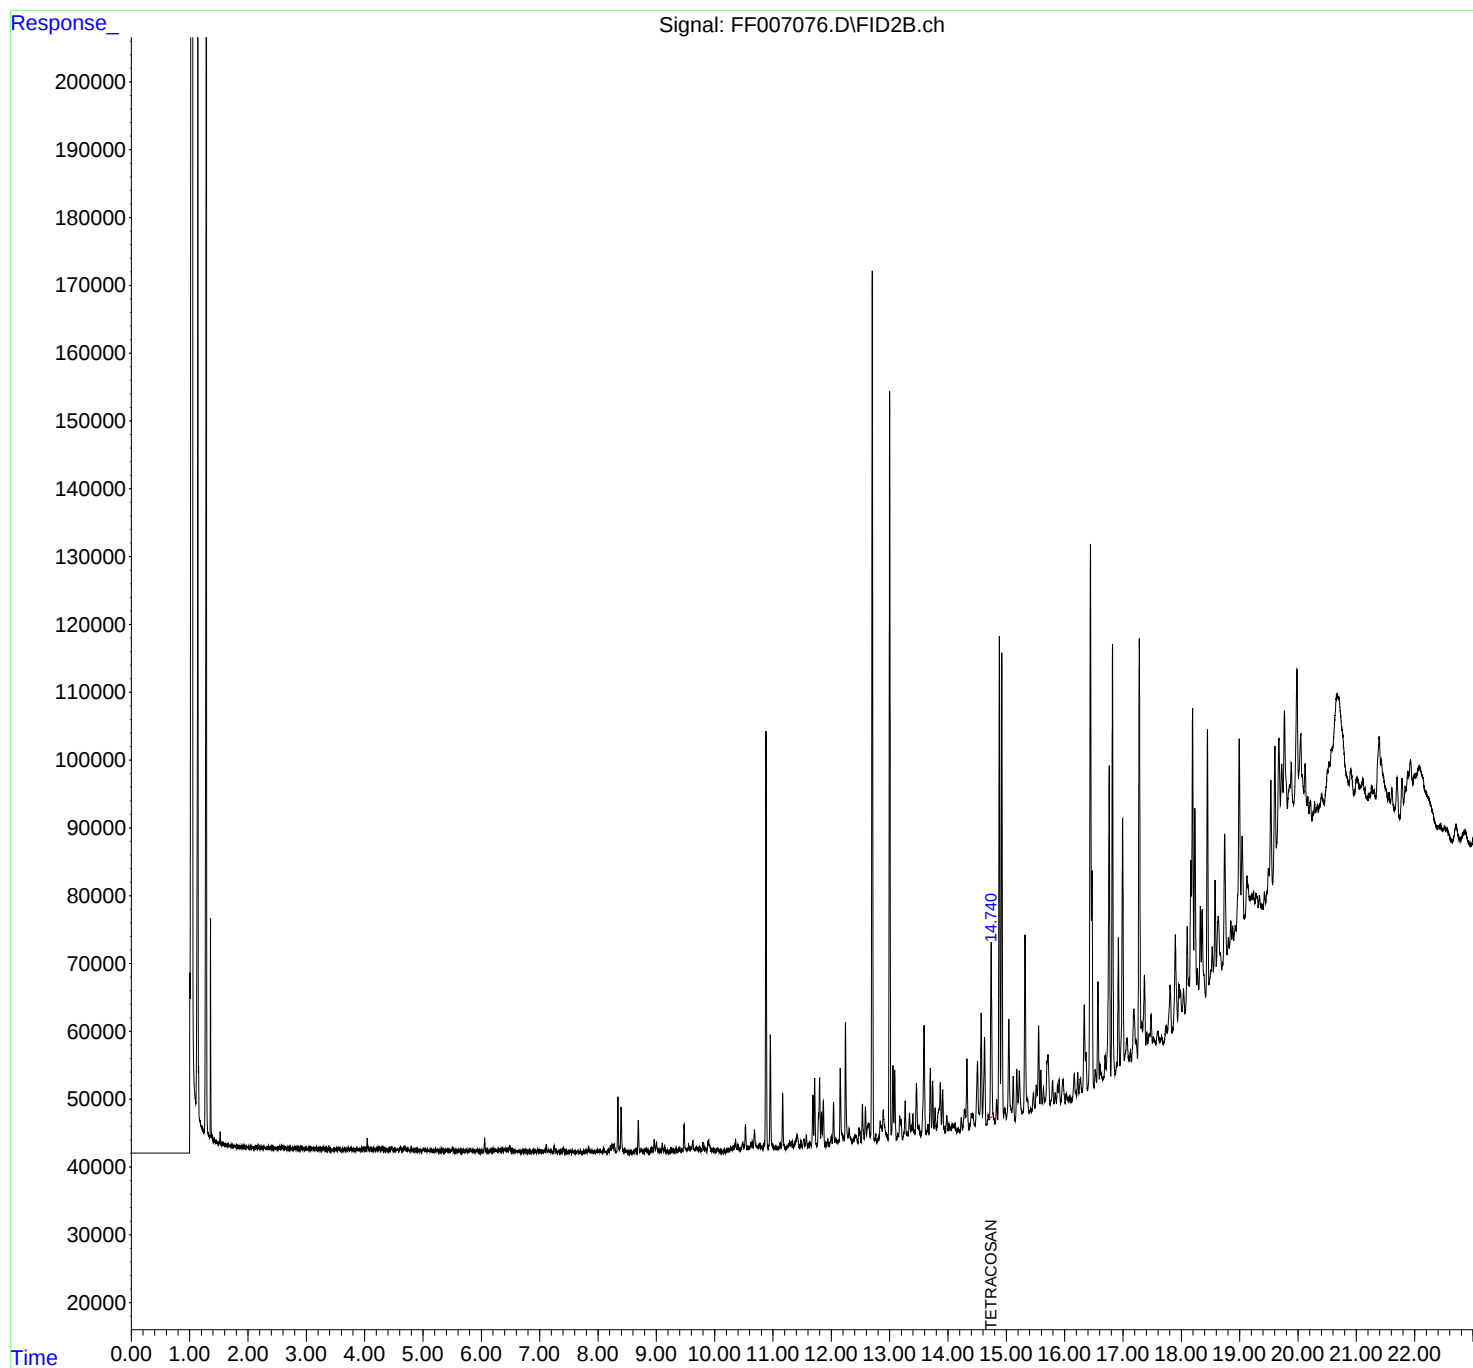

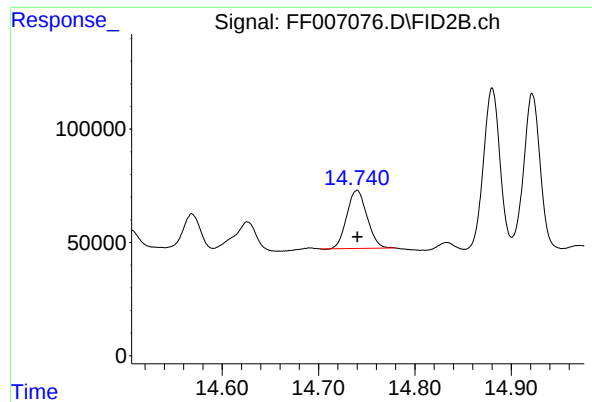

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: 0.000 min
Response: 372597
Conc: 3.17 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-A-LOT-11