

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
 Data File : FF012894.D
 Signal(s) : FID2B.ch
 Acq On : 19 Jun 2023 12:55
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 02:43:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.693	1551668	11.906 ug/ml
12) N-OCTACOSANE	17.128	1738394	13.564 ug/ml
13) N-TRIACONTANE	18.017	69763	0.541 ug/ml
14) N-DOTRIACONTANE	18.846	106693	0.844 ug/ml
15) N-TETRATRIACONTANE	19.623	138402	1.165 ug/ml
16) N-HEXATRIACONTANE	20.364	247461	2.061 ug/ml
17) N-OCTATRIACONTANE	21.090	417653	3.590 ug/ml
18) N-TETRACONTANE	21.976	574135	4.615 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012894.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2023 12:55
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 02:43:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

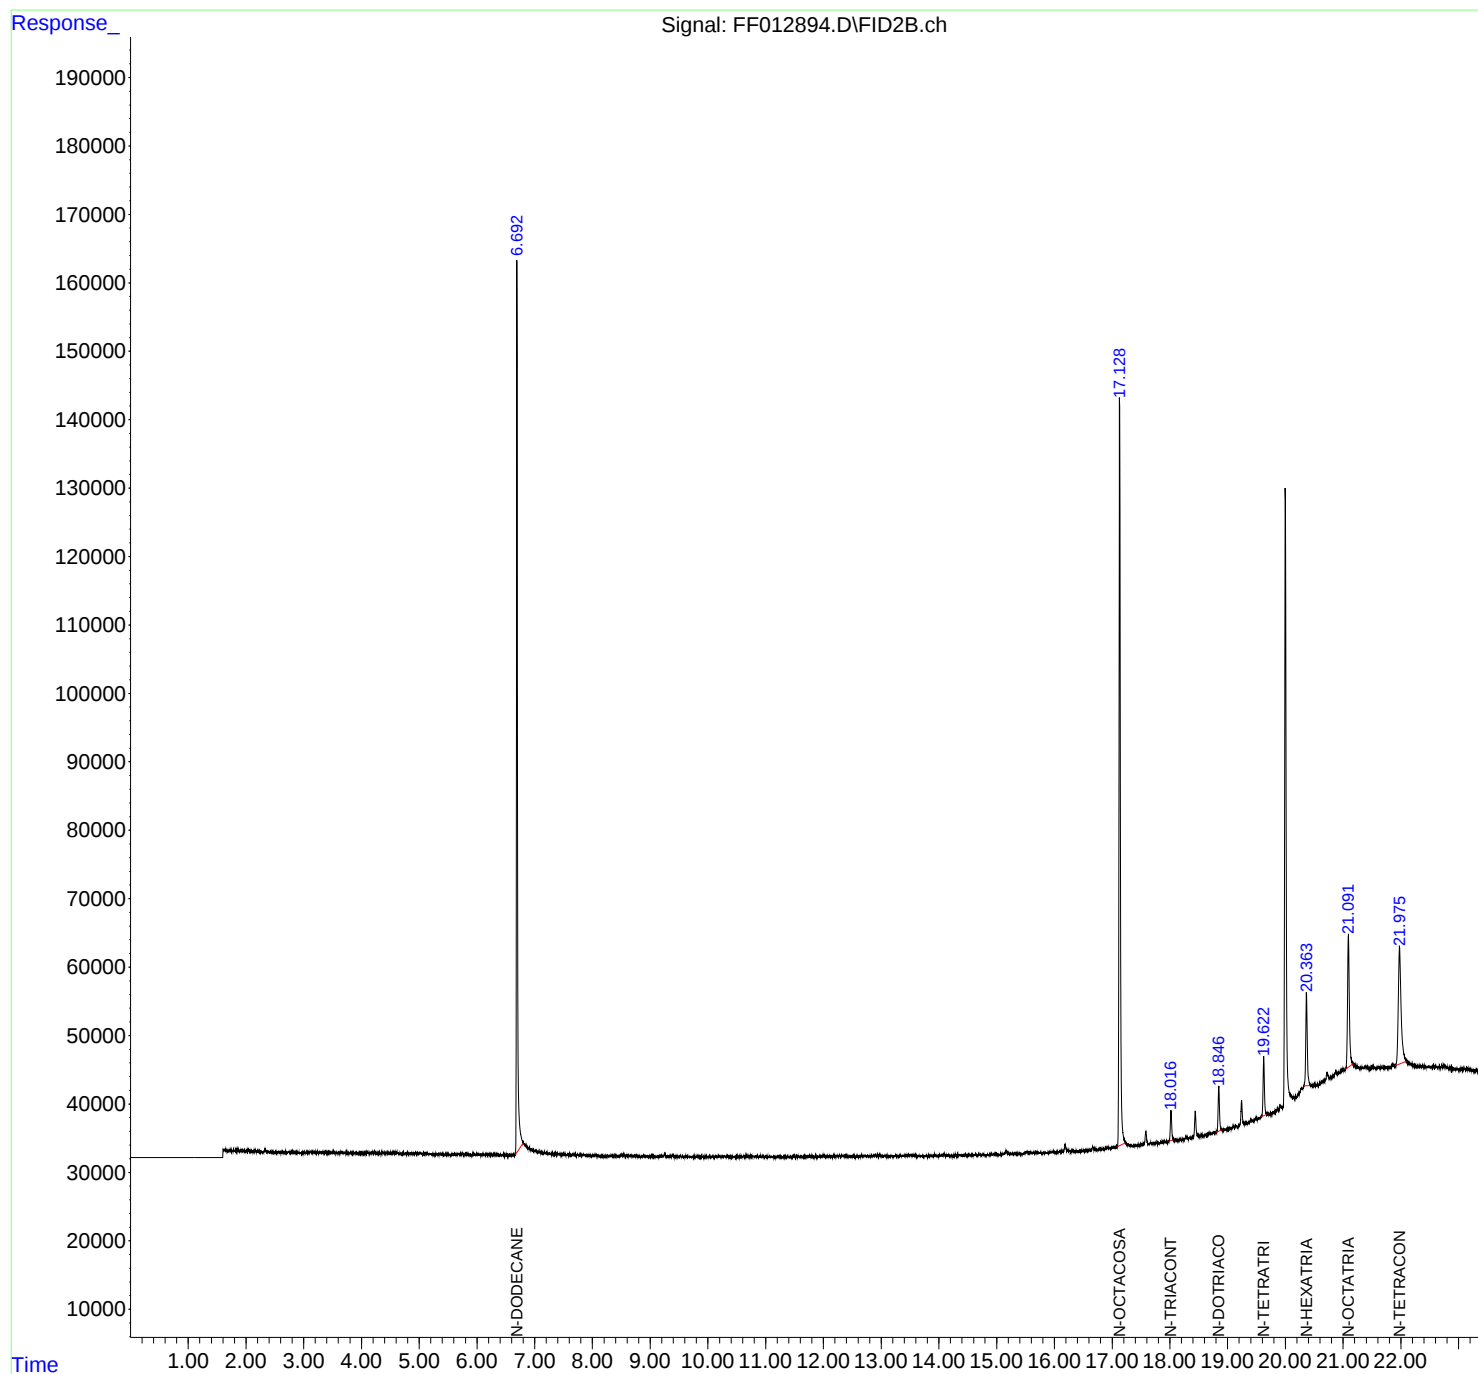


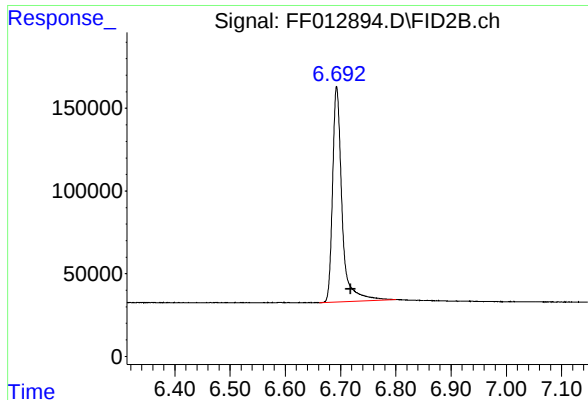

#3 N-DODECANE


R.T.: 6.693 min
Delta R.T.: -0.025 min
Response: 1551668
Conc: 11.91 ug/ml

Instrument :
FID_F
ClientSampleId :

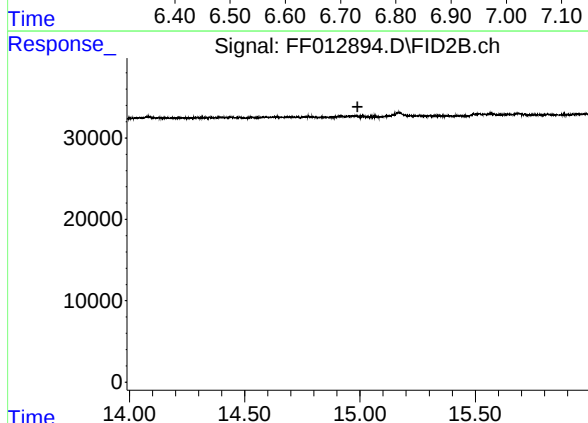


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.989 min
Response: 0
Conc: N.D.

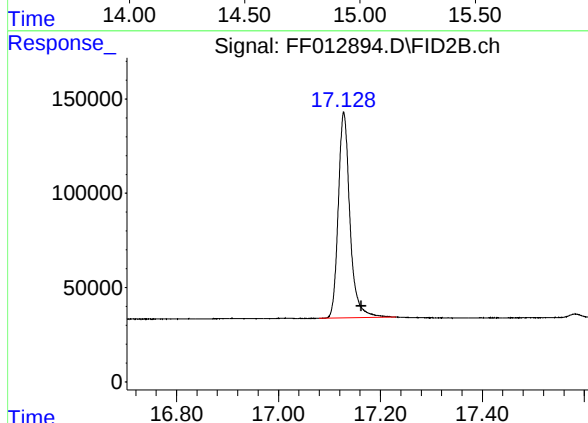


#12 N-OCTACOSANE

R.T.: 17.128 min
Delta R.T.: -0.035 min
Response: 1738394
Conc: 13.56 ug/ml

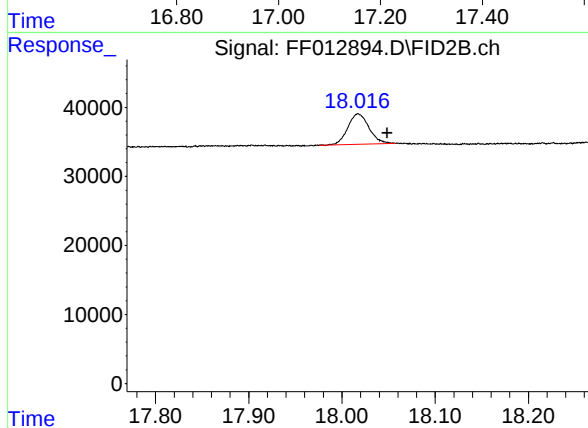

#13 N-TRIACONTANE


R.T.: 18.017 min
Delta R.T.: -0.031 min
Response: 69763
Conc: 0.54 ug/ml

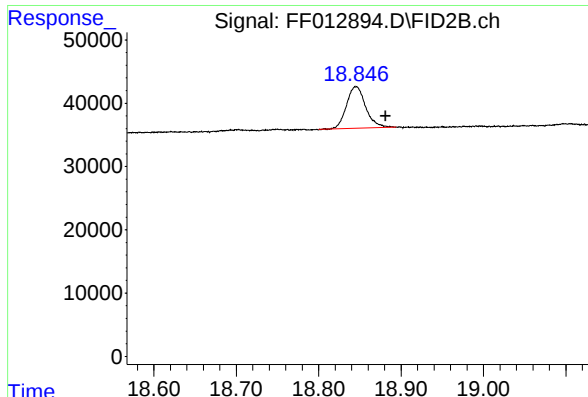

#14 N-DOTRIACONTANE


R.T.: 18.846 min
Delta R.T.: -0.036 min
Response: 106693
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

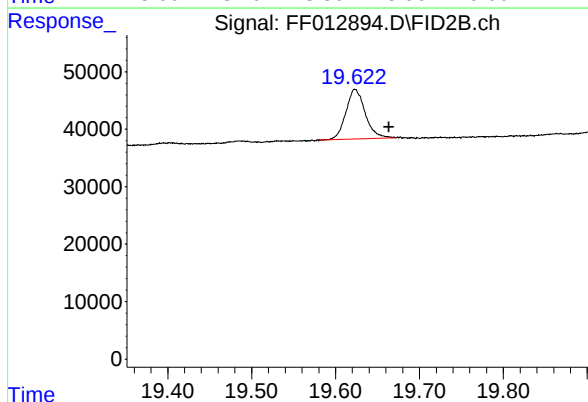


#15 N-TETRATRIACONTANE

R.T.: 19.623 min
Delta R.T.: -0.040 min
Response: 138402
Conc: 1.16 ug/ml

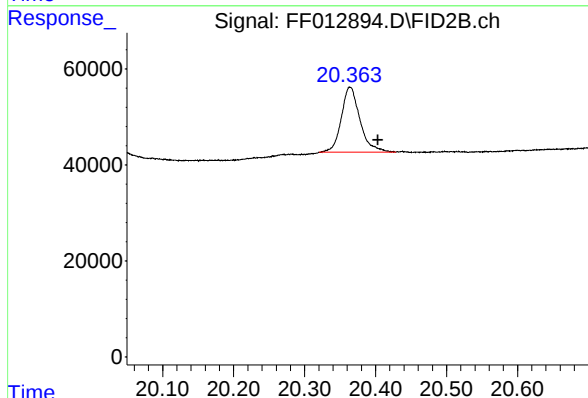


#16 N-HEXATRIACONTANE

R.T.: 20.364 min
Delta R.T.: -0.039 min
Response: 247461
Conc: 2.06 ug/ml

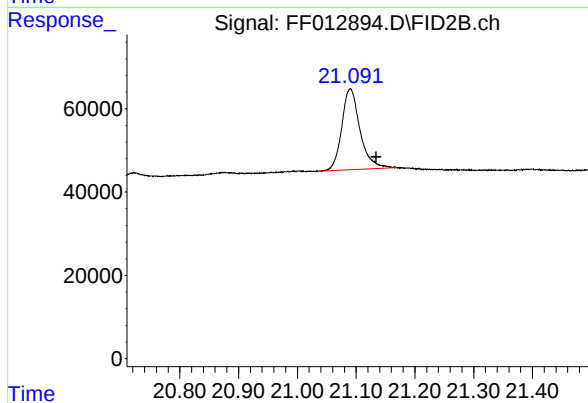

#17 N-OCTATRIACONTANE

R.T.: 21.090 min
Delta R.T.: -0.044 min
Response: 417653
Conc: 3.59 ug/ml

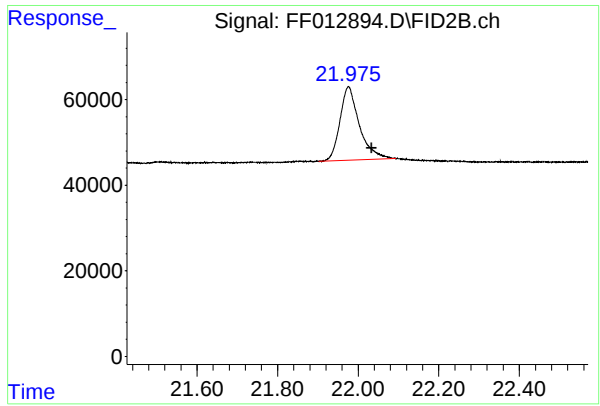

#18 N-TETRACONTANE

R.T.: 21.976 min
Delta R.T.: -0.057 min
Response: 574135
Conc: 4.61 ug/ml

Instrument :
FID_F
ClientSampleId :