

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
 Data File : FF012906.D
 Signal(s) : FID2B.ch
 Acq On : 19 Jun 2023 22:07
 Operator : YP\AJ
 Sample : 03289-11
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 02:45:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.955	1406663	12.046 ug/ml
Target Compounds			
7) N-EICOSANE	12.951f	196559	1.435 ug/ml
10) N-TETRACOSANE	15.178	149007	1.127 ug/ml
12) N-OCTACOSANE	17.123	117259	0.915 ug/ml
13) N-TRIACONTANE	18.008	131785	1.022 ug/ml
14) N-DOTRIACONTANE	18.838	322675	2.553 ug/ml
15) N-TETRATRIACONTANE	19.620	45252	0.381 ug/ml
16) N-HEXATRIACONTANE	20.355	88554	0.737 ug/ml
17) N-OCTATRIACONTANE	21.078f	95779	0.823 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012906.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2023 22:07
Operator : YP\AJ
Sample : 03289-11
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 02:45:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

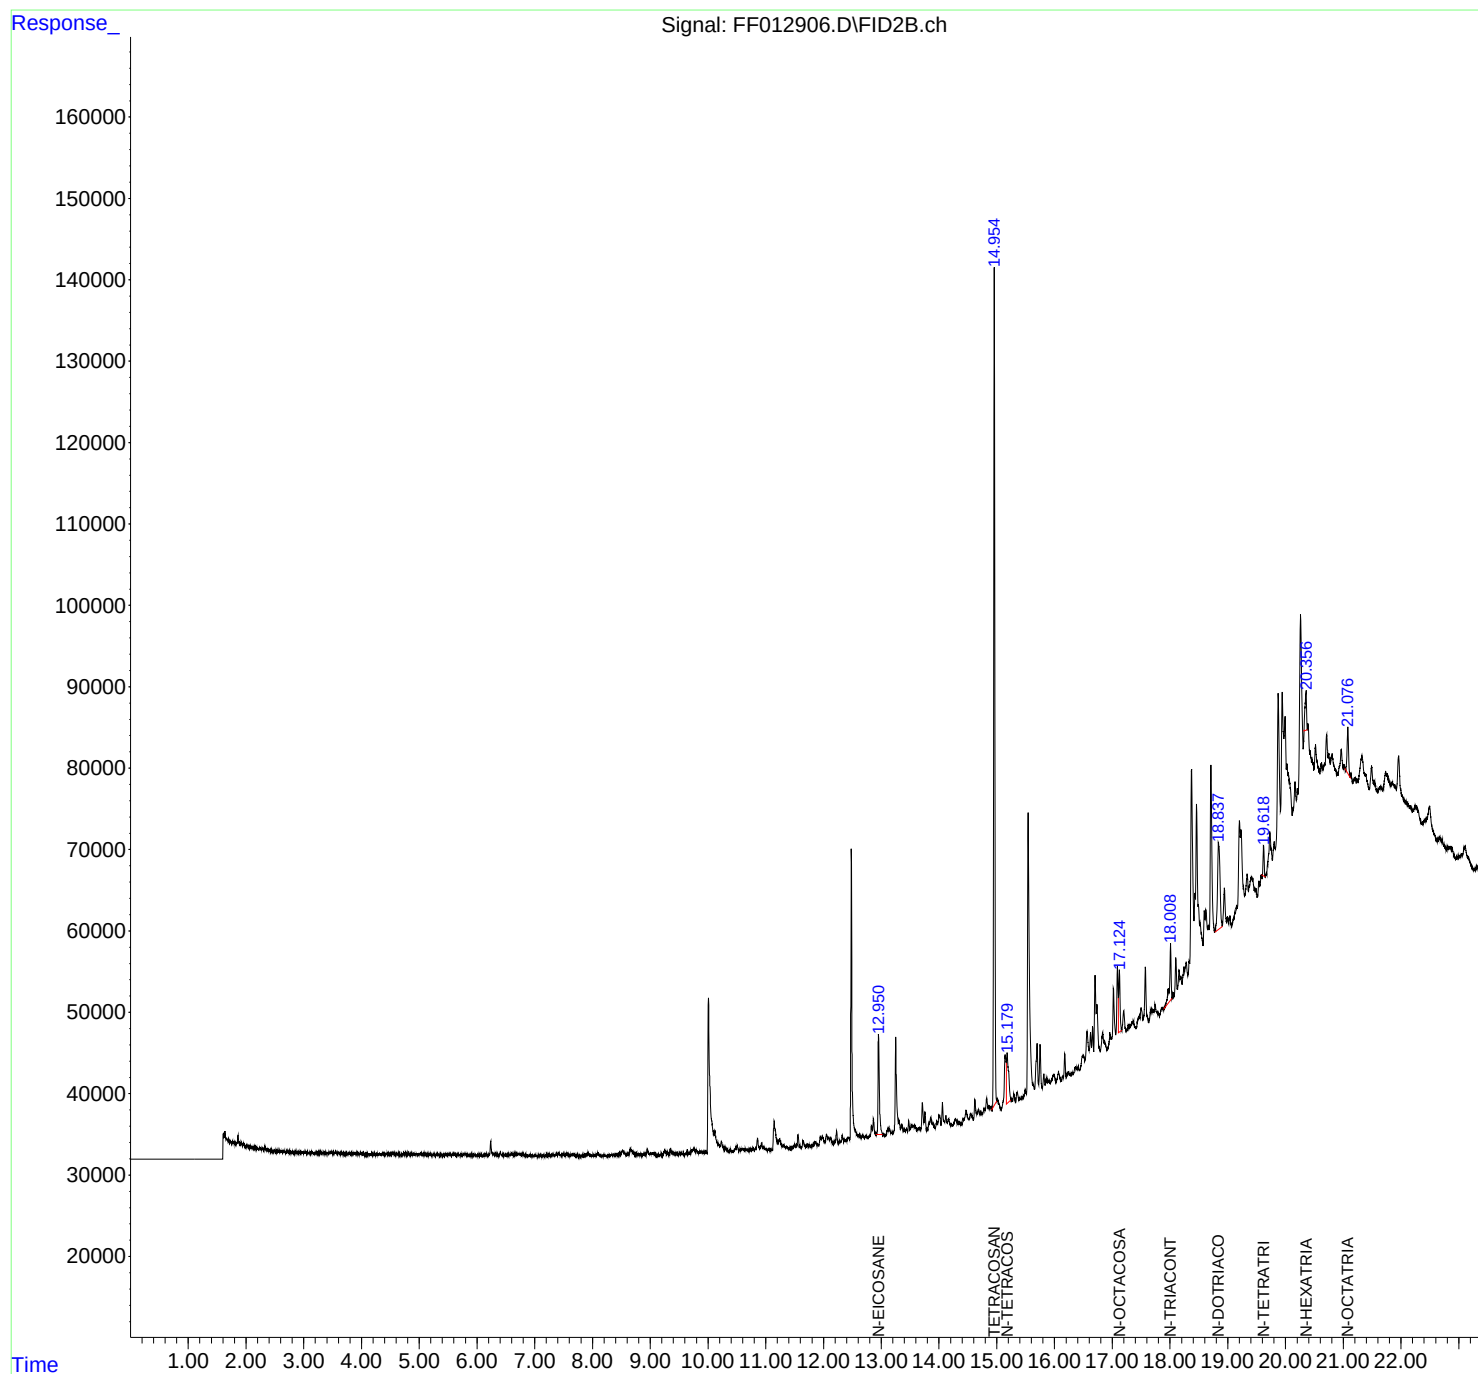


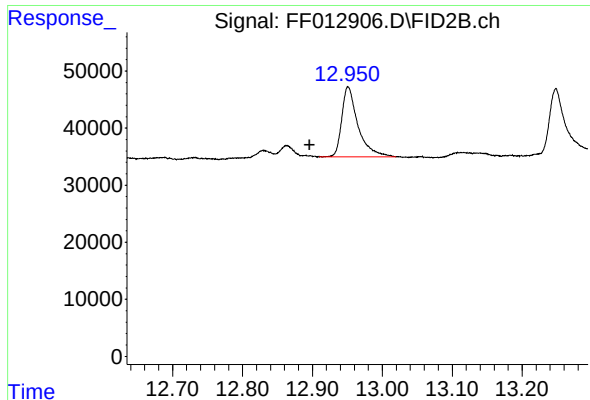

#7 N-EICOSANE


R.T.: 12.951 min
Delta R.T.: 0.055 min
Response: 196559
Conc: 1.44 ug/ml

Instrument :
FID_F
ClientSampleId :

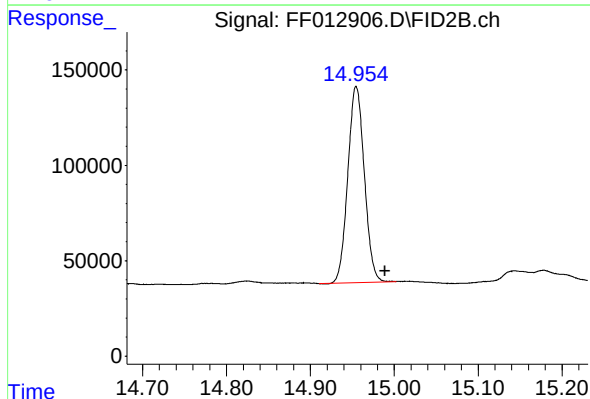


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.955 min
Delta R.T.: -0.035 min
Response: 1406663
Conc: 12.05 ug/ml

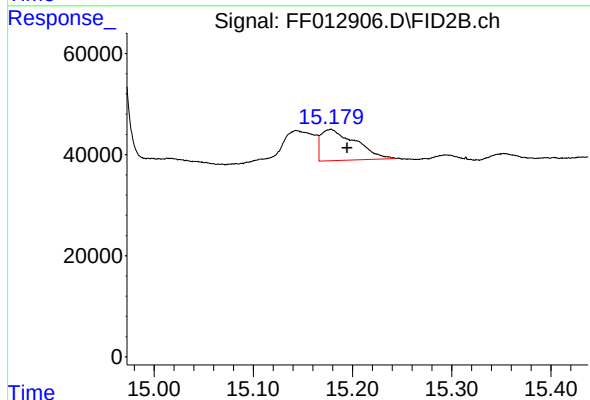


#10 N-TETRACOSANE

R.T.: 15.178 min
Delta R.T.: -0.016 min
Response: 149007
Conc: 1.13 ug/ml

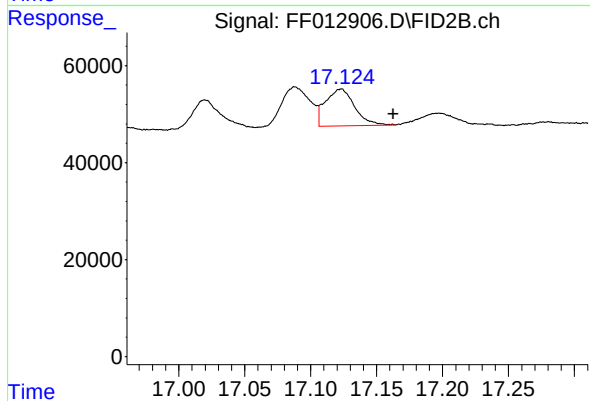

#12 N-OCTACOSANE


R.T.: 17.123 min
Delta R.T.: -0.040 min
Response: 117259
Conc: 0.91 ug/ml

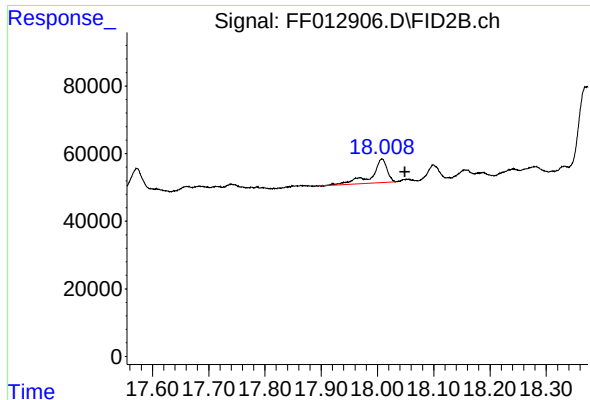

#13 N-TRIACONTANE


R.T.: 18.008 min
Delta R.T.: -0.040 min
Response: 131785
Conc: 1.02 ug/ml

Instrument :
FID_F
ClientSampleId :

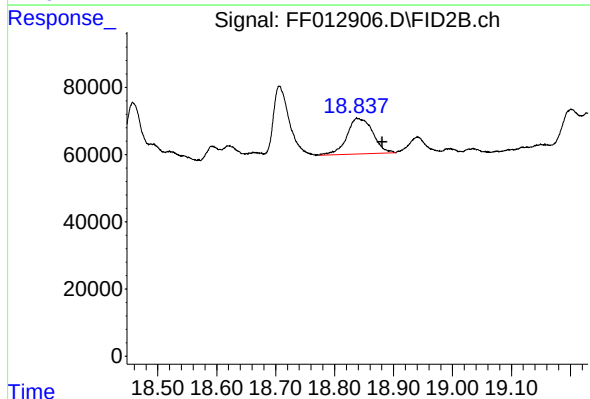


#14 N-DOTRIACONTANE

R.T.: 18.838 min
Delta R.T.: -0.043 min
Response: 322675
Conc: 2.55 ug/ml

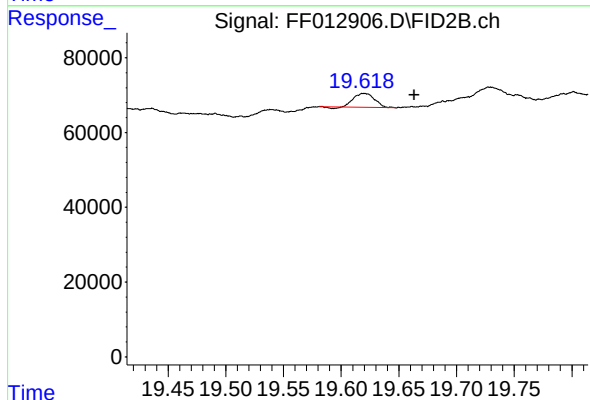


#15 N-TETRATRIACONTANE

R.T.: 19.620 min
Delta R.T.: -0.044 min
Response: 45252
Conc: 0.38 ug/ml

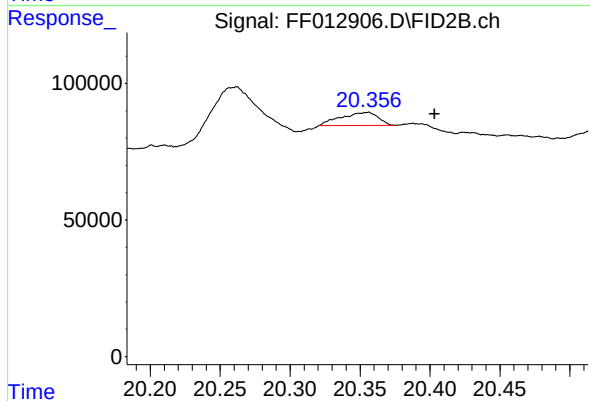

#16 N-HEXATRIACONTANE

R.T.: 20.355 min
Delta R.T.: -0.048 min
Response: 88554
Conc: 0.74 ug/ml

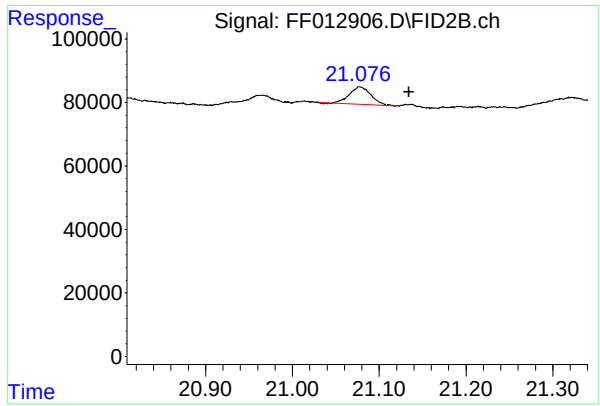

#17 N-OCTATRIACONTANE

R.T.: 21.078 min
Delta R.T.: -0.057 min
Response: 95779
Conc: 0.82 ug/ml

Instrument :

FID_F

ClientSampleId :