

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
 Data File : FF012911.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2023 00:34
 Operator : YP\AJ
 Sample : 03289-24
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 03:47:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.955	1373888	11.765 ug/ml
Target Compounds			
7) N-EICOSANE	12.955f	119775	0.875 ug/ml
10) N-TETRACOSANE	15.199	104994	0.794 ug/ml
11) N-HEXACOSANE	16.177	49388	0.382 ug/ml
12) N-OCTACOSANE	17.171	59638	0.465 ug/ml
13) N-TRIACONTANE	18.009	95100	0.738 ug/ml
14) N-DOTRIACONTANE	18.836	124995	0.989 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012911.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2023 00:34
Operator : YP\AJ
Sample : 03289-24
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 03:47:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

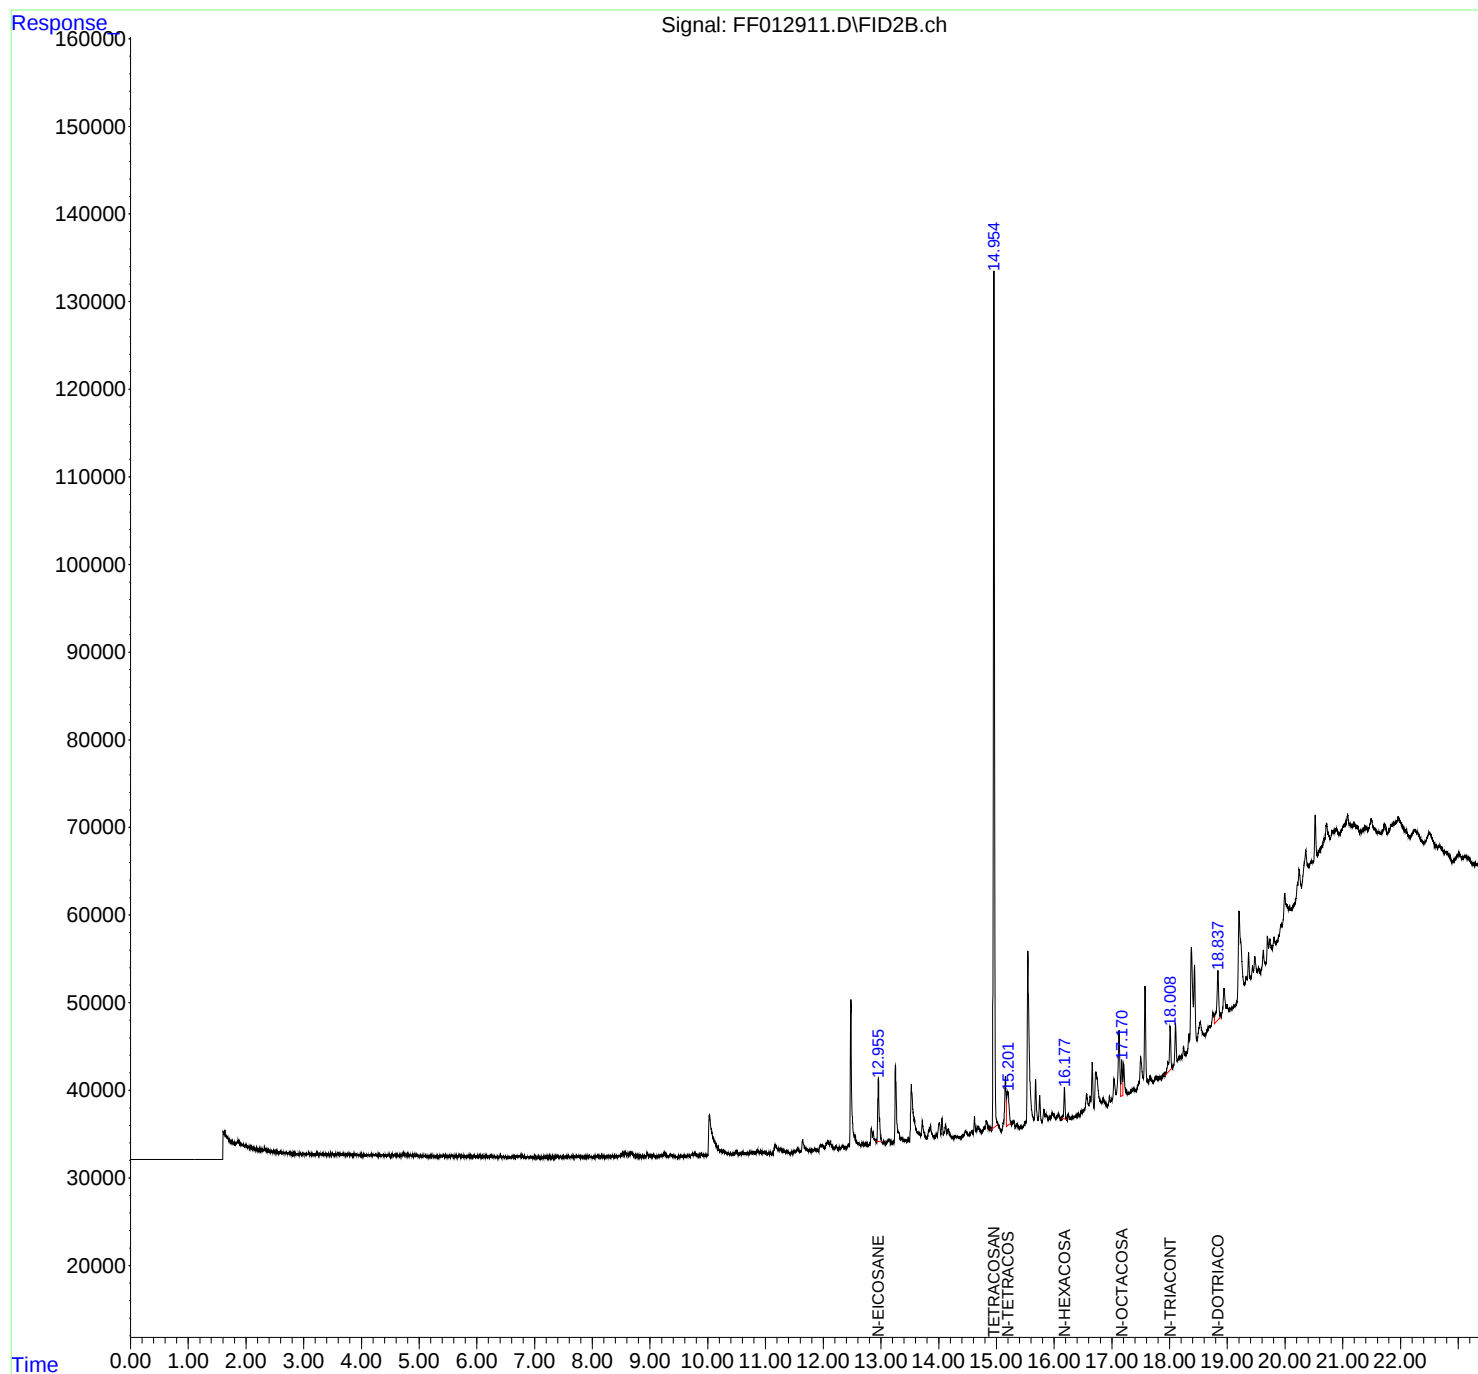


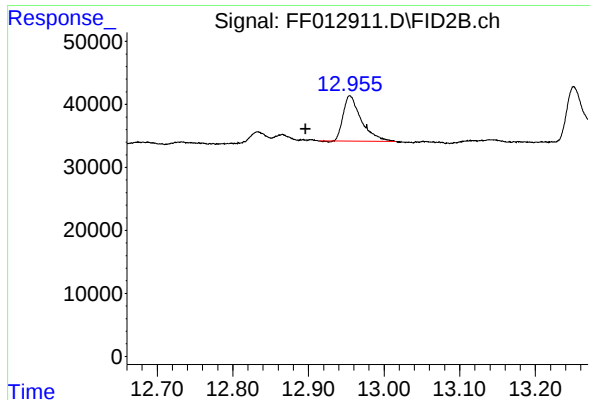

#7 N-EICOSANE


R.T.: 12.955 min
Delta R.T.: 0.059 min
Response: 119775
Conc: 0.87 ug/ml

Instrument :
FID_F
ClientSampleId :

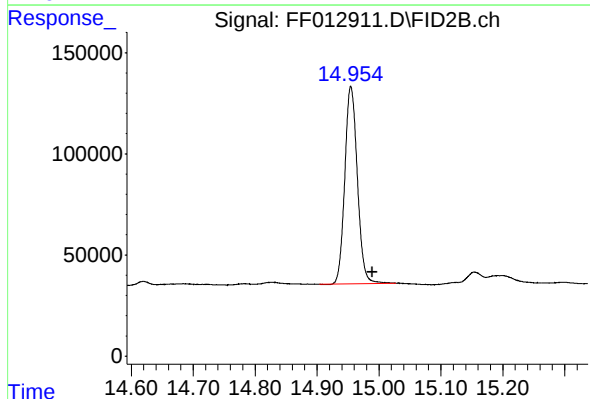


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.955 min
Delta R.T.: -0.034 min
Response: 1373888
Conc: 11.77 ug/ml

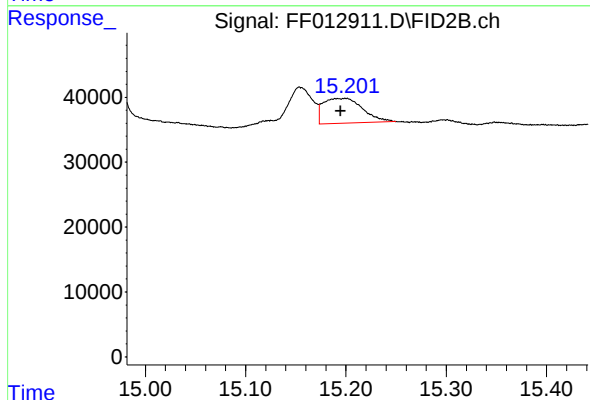


#10 N-TETRACOSANE

R.T.: 15.199 min
Delta R.T.: 0.005 min
Response: 104994
Conc: 0.79 ug/ml

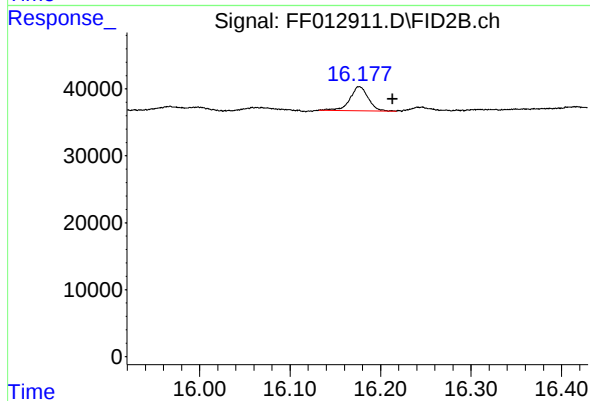

#11 N-HEXACOSANE


R.T.: 16.177 min
Delta R.T.: -0.037 min
Response: 49388
Conc: 0.38 ug/ml

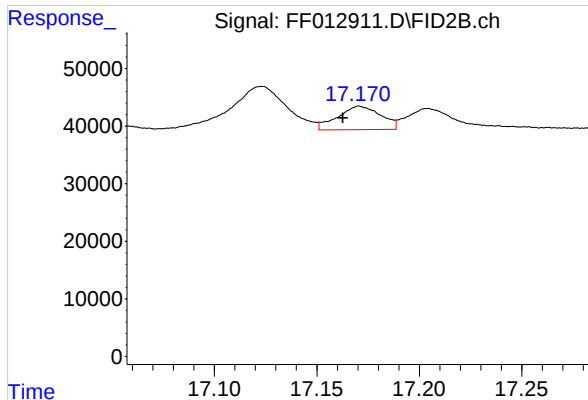

#12 N-OCTACOSANE


R.T.: 17.171 min
Delta R.T.: 0.008 min
Response: 59638
Conc: 0.47 ug/ml

Instrument :
FID_F
ClientSampleId :

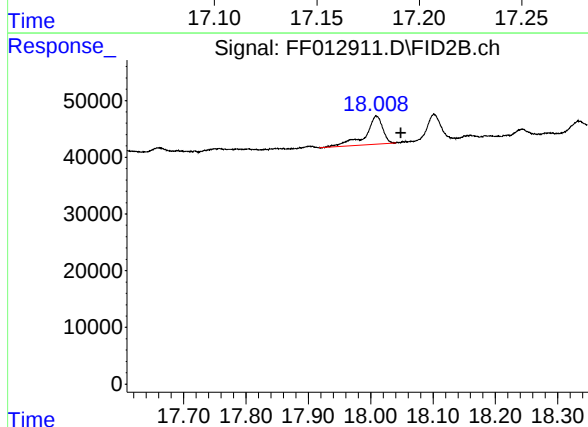

#13 N-TRIACONTANE

R.T.: 18.009 min
Delta R.T.: -0.039 min
Response: 95100
Conc: 0.74 ug/ml

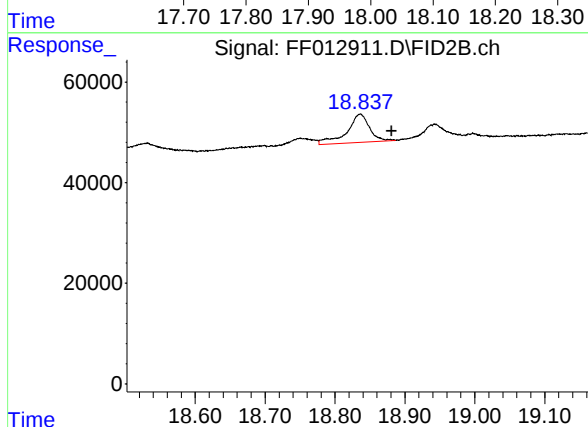

#14 N-DOTRIACONTANE

R.T.: 18.836 min
Delta R.T.: -0.045 min
Response: 124995
Conc: 0.99 ug/ml