

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
 Data File : FF012916.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2023 08:22
 Operator : YP\AJ
 Sample : 03289-09 5X
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 11:34:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.999	137848	1.180 ug/ml
Target Compounds			
6) N-OCTADECANE	11.656f	90557	0.659 ug/ml
7) N-EICOSANE	12.884	103017	0.752 ug/ml
8) N-DOCOSANE	14.104	366088	2.769 ug/ml
10) N-TETRACOSANE	15.158	1975056	14.944 ug/ml
11) N-HEXACOSANE	16.219	89530	0.693 ug/ml
12) N-OCTACOSANE	17.168	578755	4.516 ug/ml
13) N-TRIACONTANE	18.008	13498	0.105 ug/ml
14) N-DOTRIACONTANE	18.853	343616	2.719 ug/ml


(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012916.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2023 08:22
Operator : YP\AJ
Sample : 03289-09 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 20 11:34:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

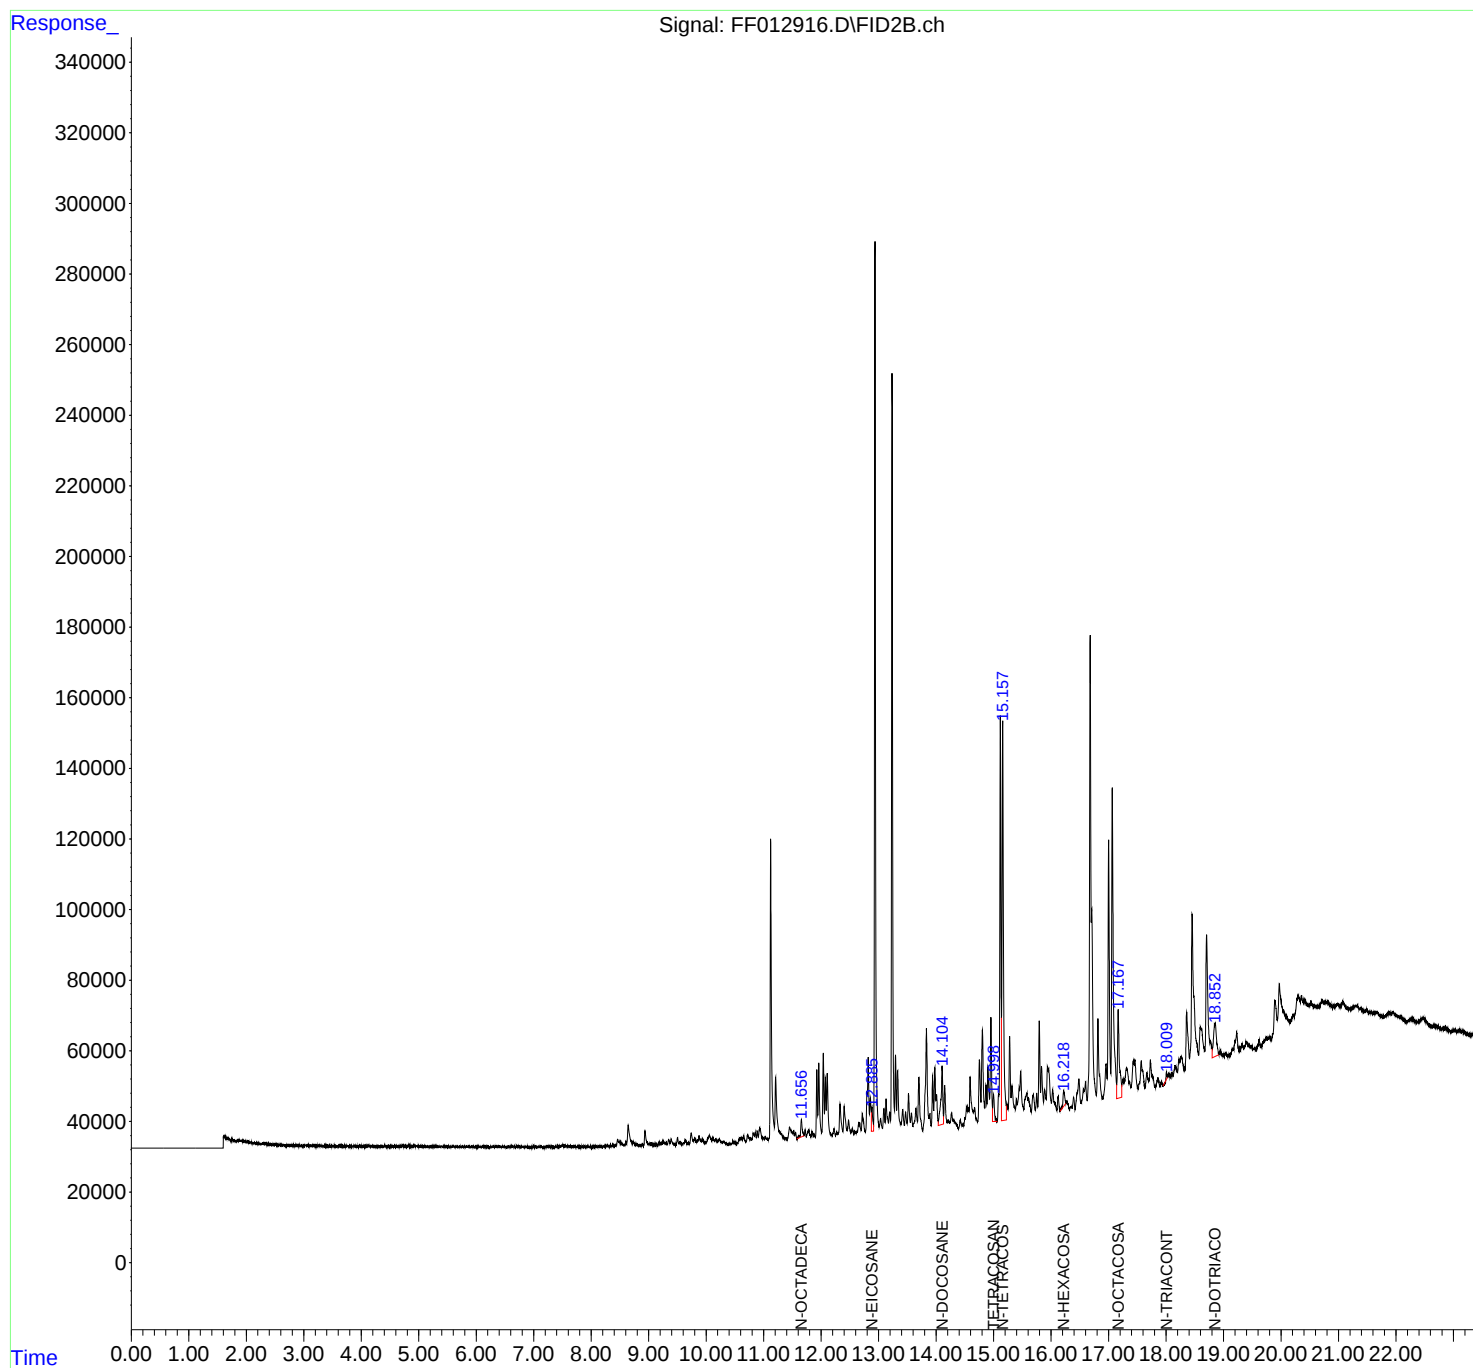


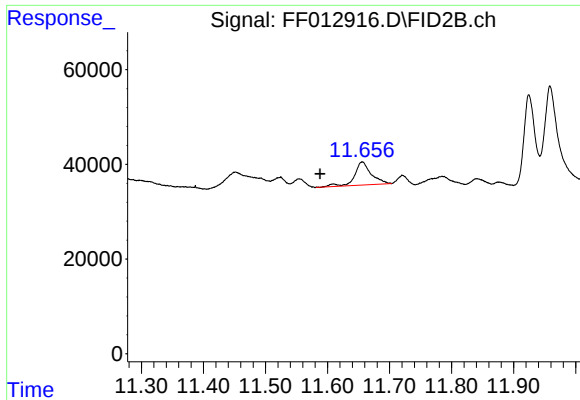

#6 N-OCTADECANE


R.T.: 11.656 min
Delta R.T.: 0.068 min
Response: 90557
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

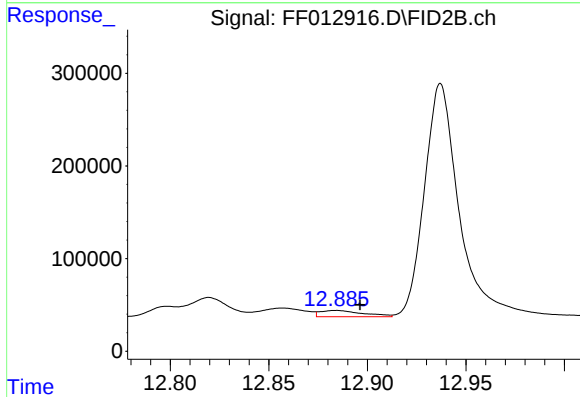


#7 N-EICOSANE

R.T.: 12.884 min
Delta R.T.: -0.012 min
Response: 103017
Conc: 0.75 ug/ml

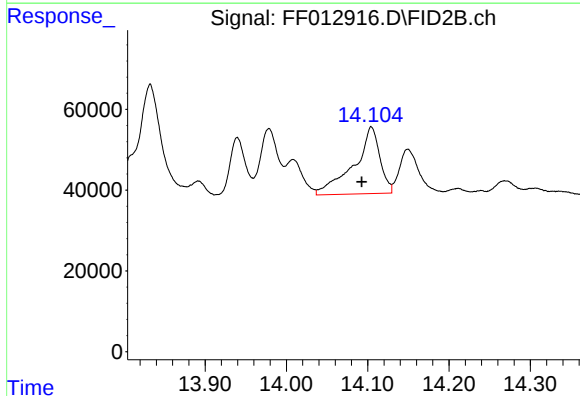


#8 N-DOCOSANE

R.T.: 14.104 min
Delta R.T.: 0.012 min
Response: 366088
Conc: 2.77 ug/ml

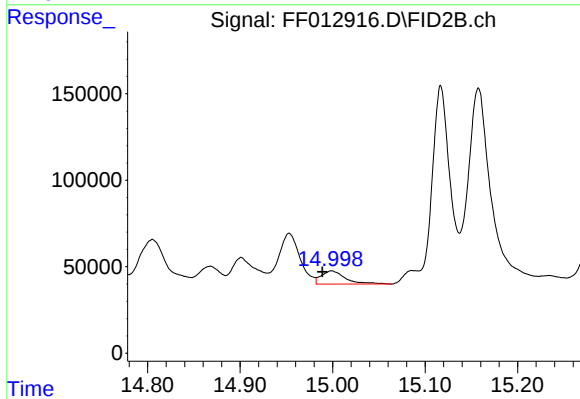

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.999 min
Delta R.T.: 0.010 min
Response: 137848
Conc: 1.18 ug/ml

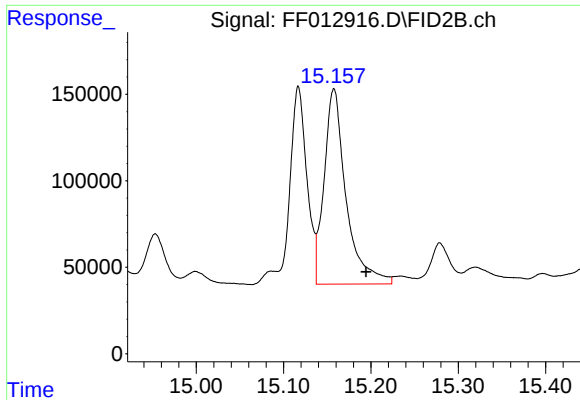

#10 N-TETRACOSANE


R.T.: 15.158 min
Delta R.T.: -0.037 min
Response: 1975056
Conc: 14.94 ug/ml

Instrument :
FID_F
ClientSampleId :

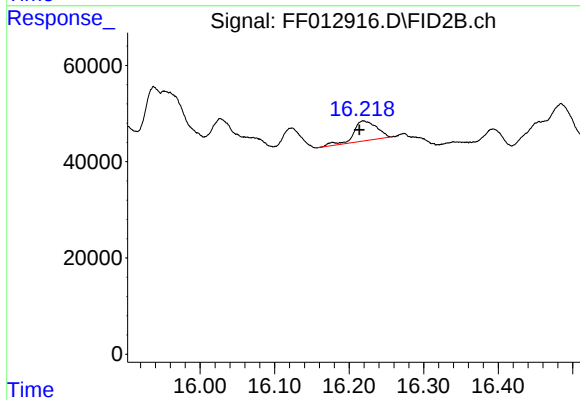


#11 N-HEXACOSANE

R.T.: 16.219 min
Delta R.T.: 0.006 min
Response: 89530
Conc: 0.69 ug/ml

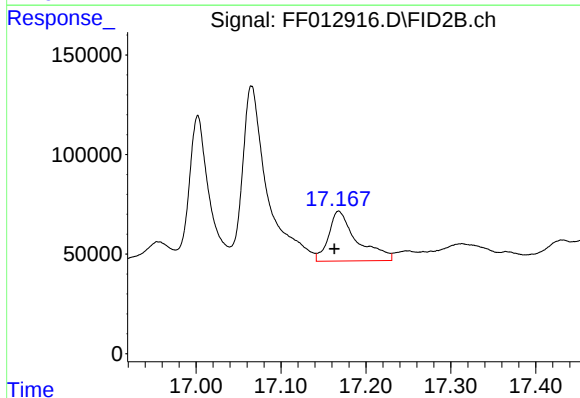


#12 N-OCTACOSANE

R.T.: 17.168 min
Delta R.T.: 0.005 min
Response: 578755
Conc: 4.52 ug/ml

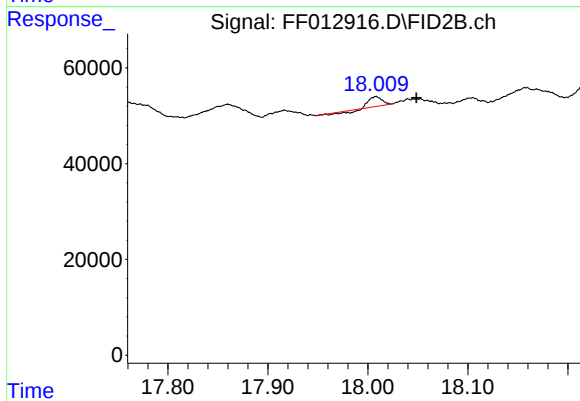

#13 N-TRIACONTANE

R.T.: 18.008 min
Delta R.T.: -0.041 min
Response: 13498
Conc: 0.10 ug/ml

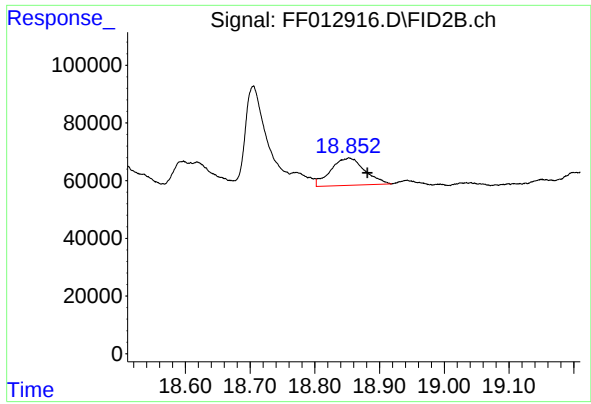

#14 N-DOTRIACONTANE

R.T.: 18.853 min
Delta R.T.: -0.029 min
Response: 343616
Conc: 2.72 ug/ml

Instrument :
FID_F
ClientSampleId :