

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012900.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2023 17:41
Operator : YP\AJ
Sample : 03282-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-NEX-002-G

Integration File: autoint1.e
Quant Time: Jun 20 02:44:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.956	1682277	14.406 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012900.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2023 17:41
Operator : YP\AJ
Sample : 03282-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-NEX-002-G

Integration File: autoint1.e
Quant Time: Jun 20 02:44:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

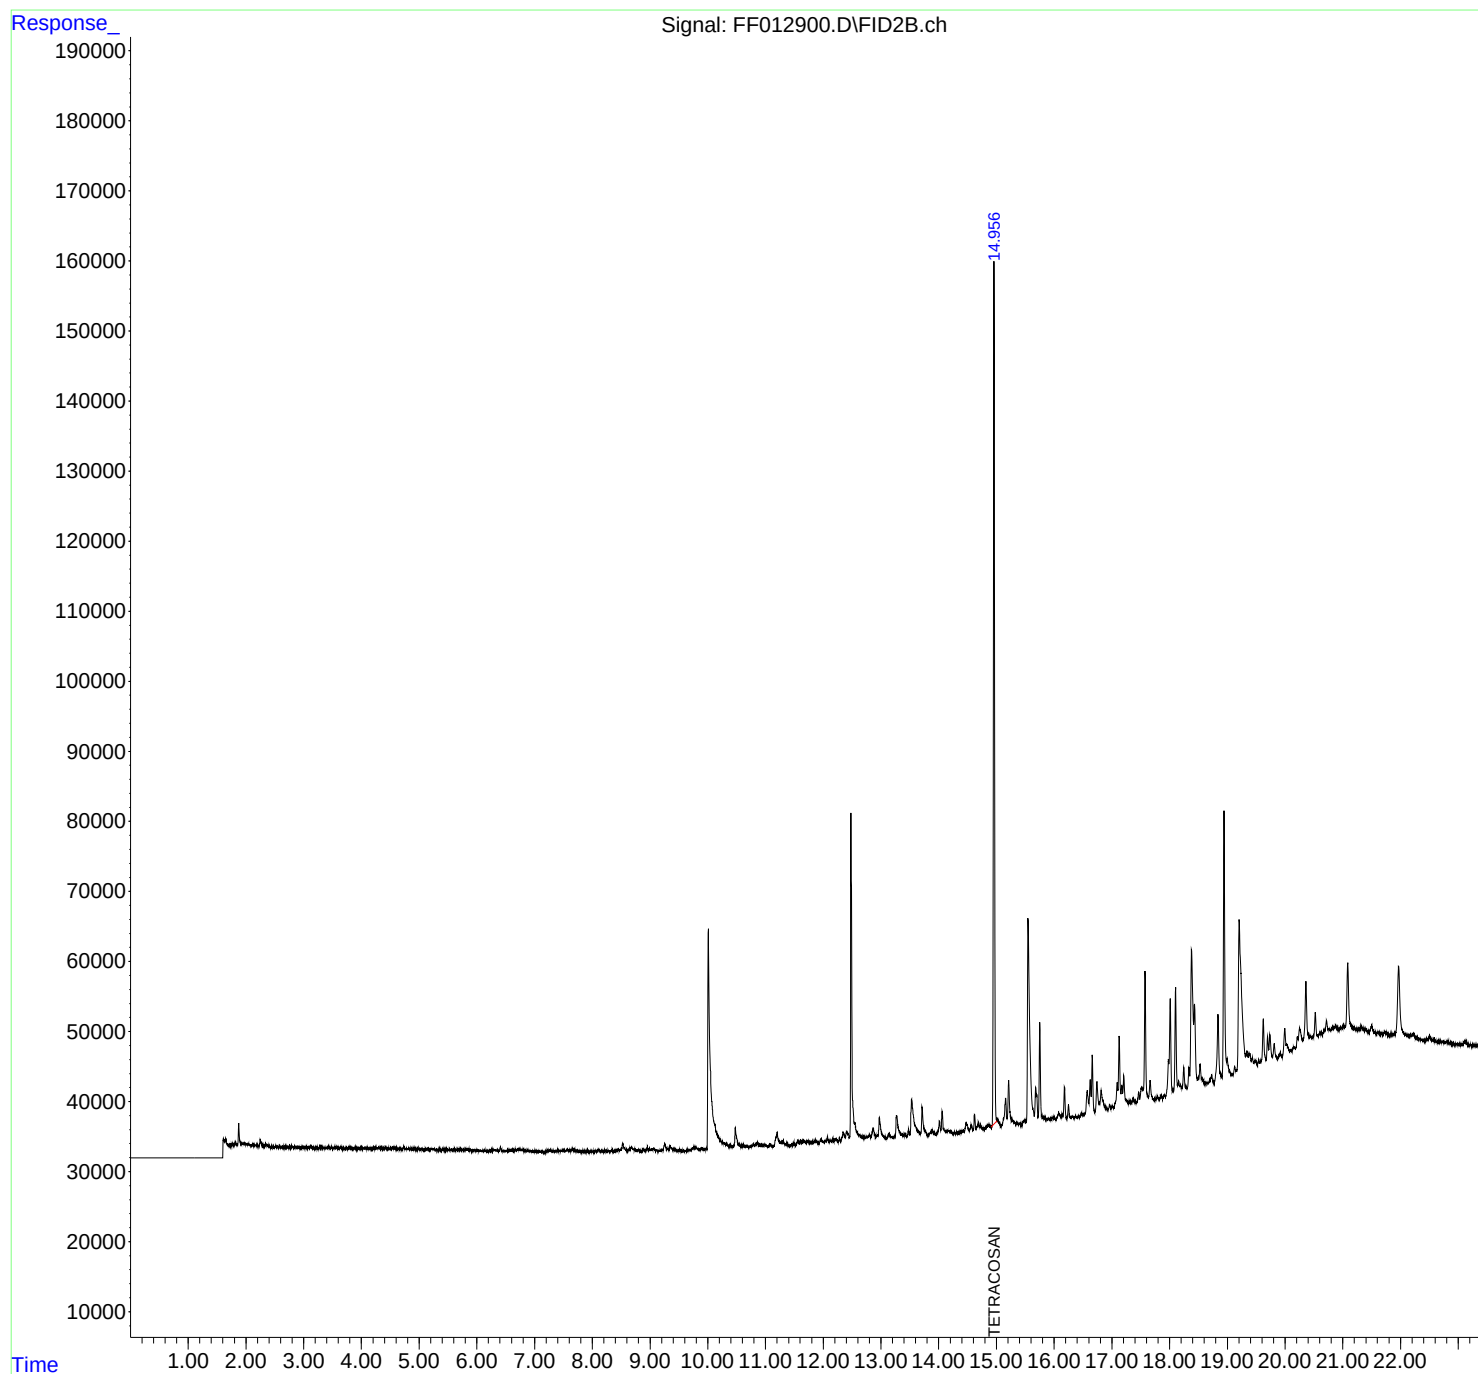

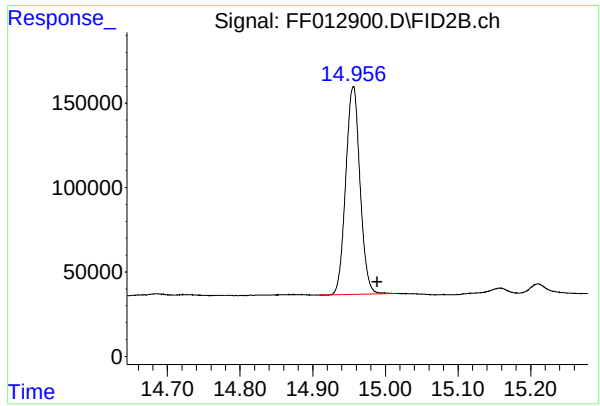

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.956 min
Delta R.T.: -0.033 min
Response: 1682277
Conc: 14.41 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-NEX-002-G