

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012905.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2023 21:37
Operator : YP\AJ
Sample : 03289-09
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-03-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

Integration File: autoint1.e
Quant Time: Jun 20 02:44:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.957	1867297	15.990 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012905.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2023 21:37
Operator : YP\AJ
Sample : 03289-09
Misc :
ALS Vial : 69 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

Integration File: autoint1.e
Quant Time: Jun 20 02:44:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

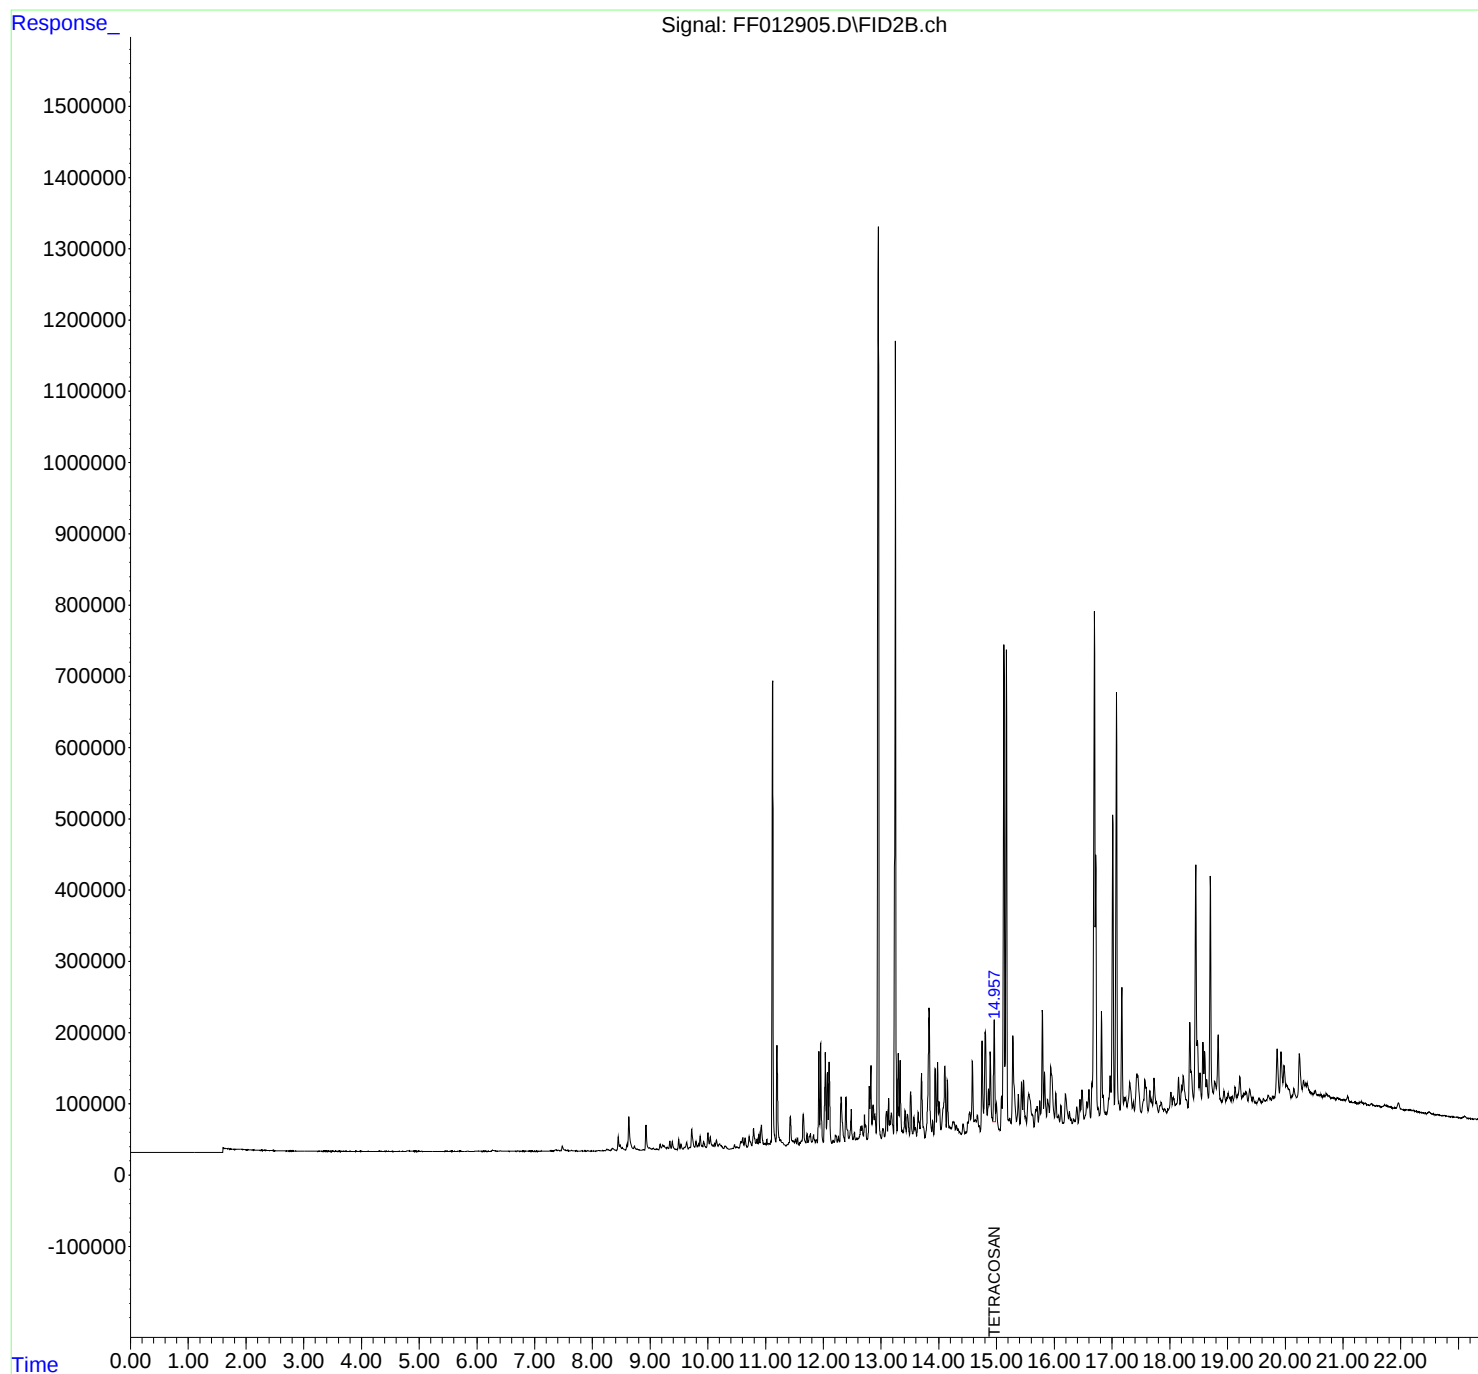

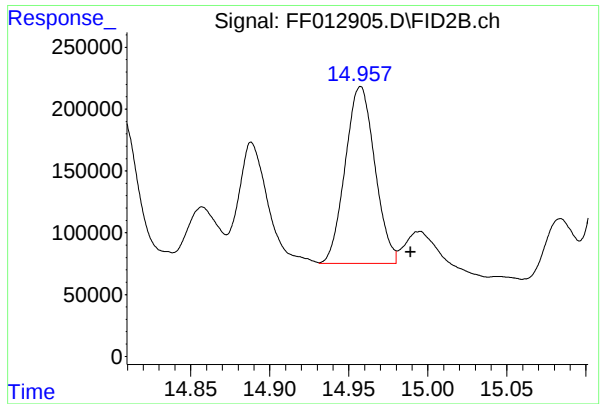

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.957 min
Delta R.T.: -0.032 min
Response: 1867297
Conc: 15.99 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-03-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023