

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012916.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2023 08:22
Operator : YP\AJ
Sample : 03289-09 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-03-COMP

Integration File: Sample.e
Quant Time: Jun 20 11:34:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.953	369026	3.160 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061923\
Data File : FF012916.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2023 08:22
Operator : YP\AJ
Sample : 03289-09 5X
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-03-COMP

Integration File: Sample.e
Quant Time: Jun 20 11:34:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

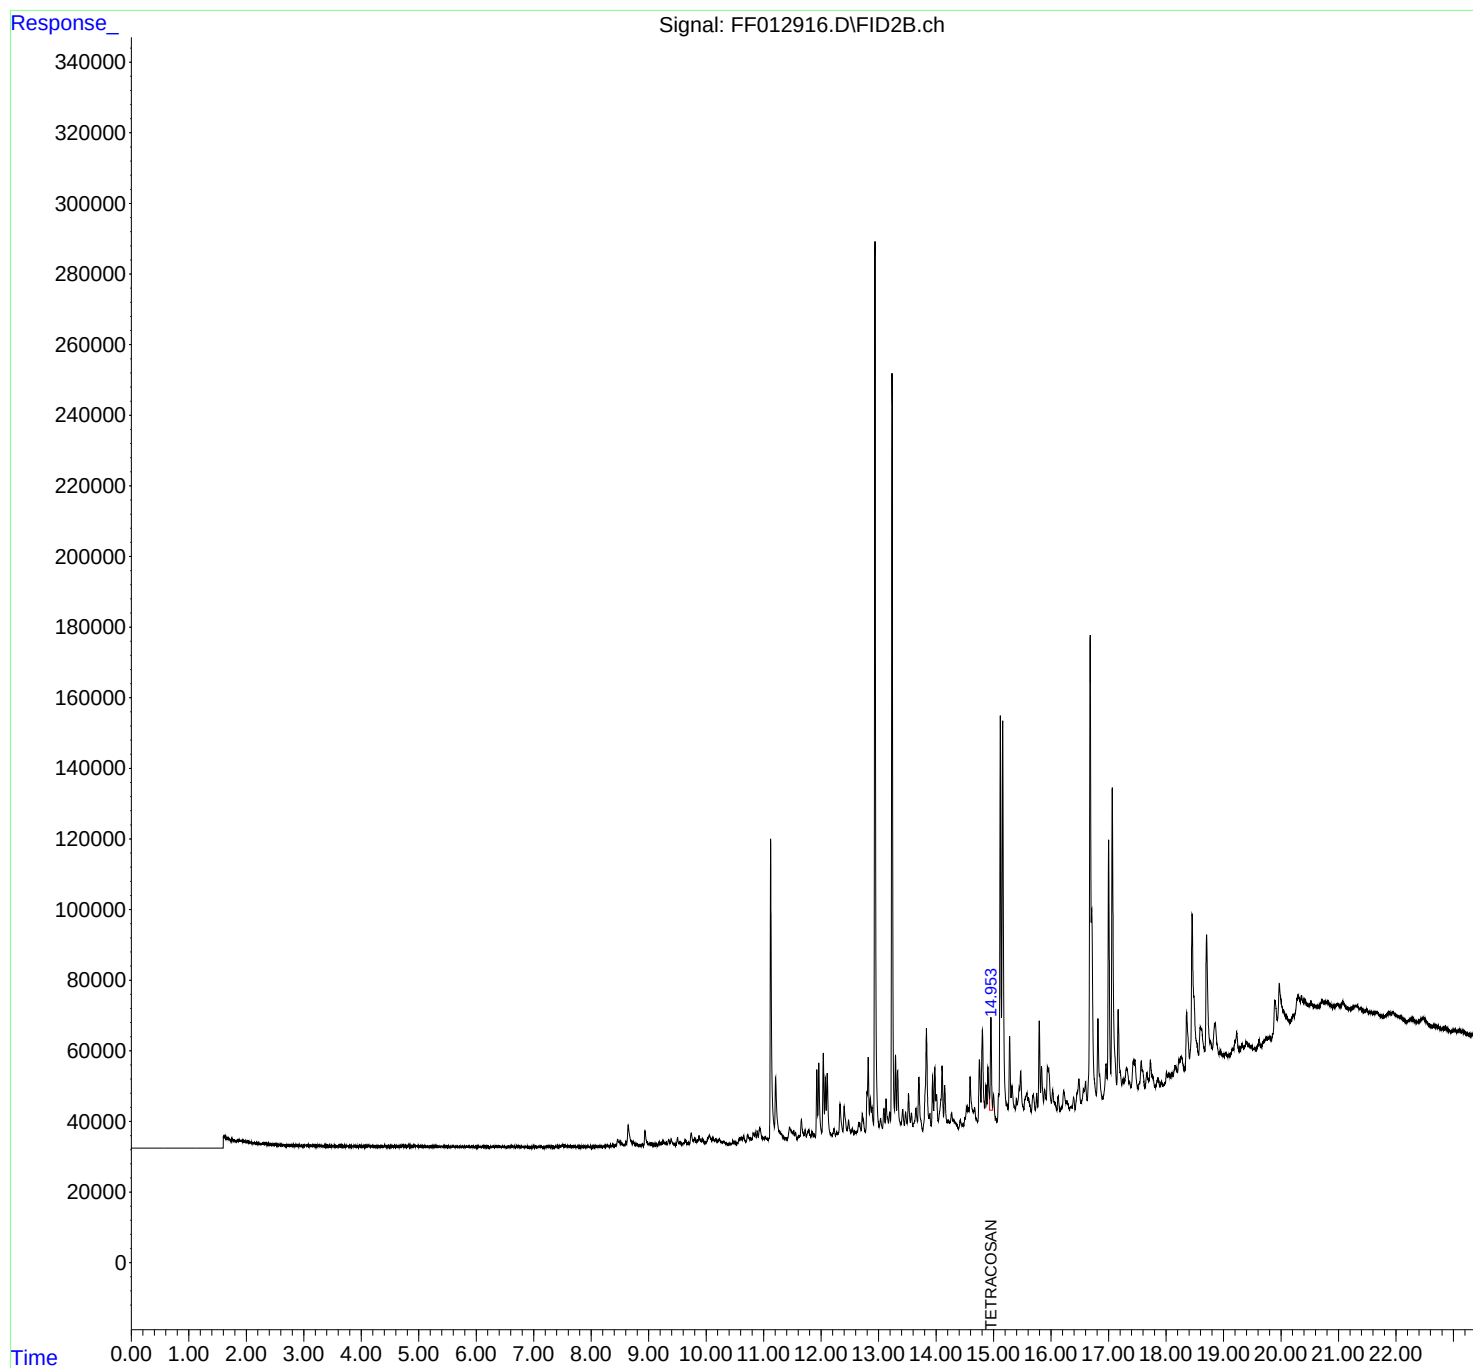

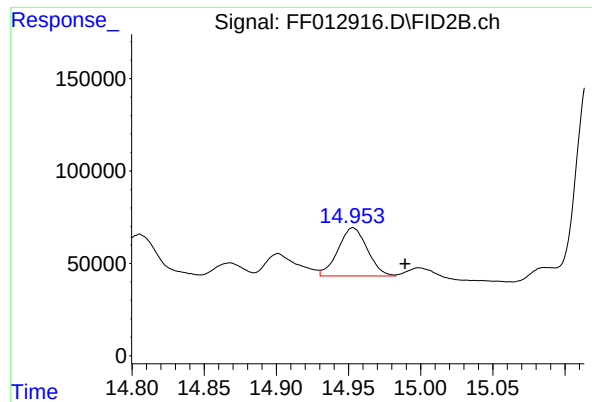

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.953 min
Delta R.T.: -0.036 min
Response: 369026
Conc: 3.16 ug/ml

Instrument :

FID_F

ClientSampleId :

SB-03-COMP