

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001028.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 11:11
 Operator : UA\AJ
 Sample : J3575-16 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:49:53 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.479	285760	2.478 ug/ml
Target Compounds			
2) N-DECANE	4.241	679882	4.852 ug/ml
3) N-DODECANE	6.254	826878	5.900 ug/ml
4) N-TETRADECANE	8.043	614441	4.413 ug/ml
5) N-HEXADECANE	9.638	327265	2.374 ug/ml
16) N-HEXATRIACONTANE	19.894	41808	0.366 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001028.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 11:11
Operator : UA\AJ
Sample : J3575-16 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:49:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

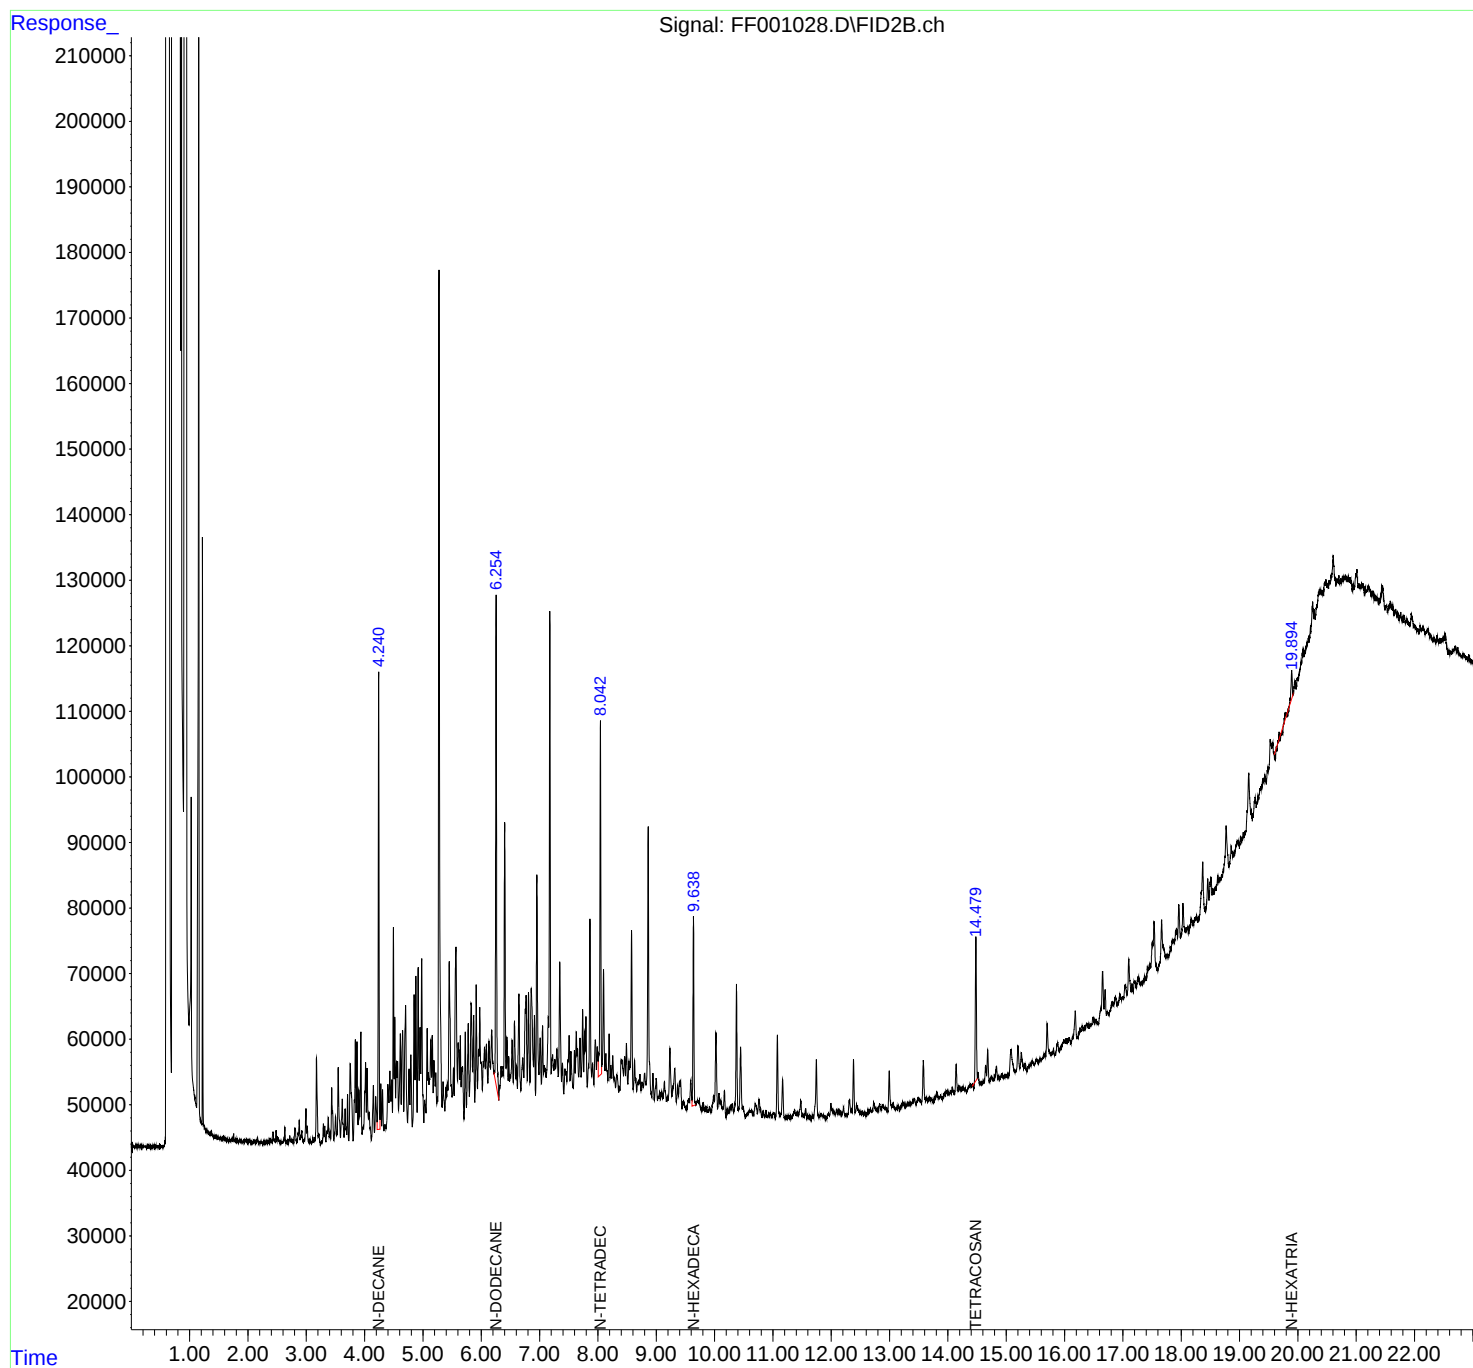


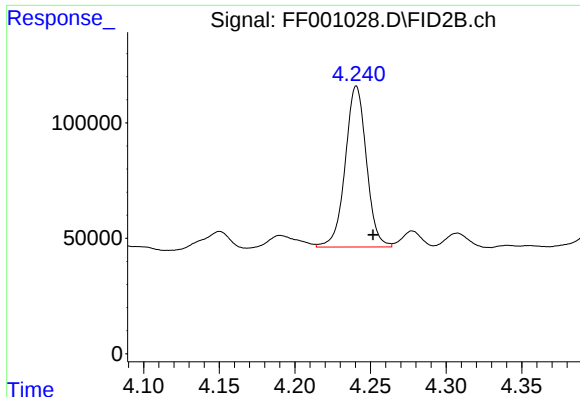

#2 N-DECANE


R.T.: 4.241 min
Delta R.T.: -0.011 min
Response: 679882
Conc: 4.85 ug/ml

Instrument :
FID_F
ClientSampleId :

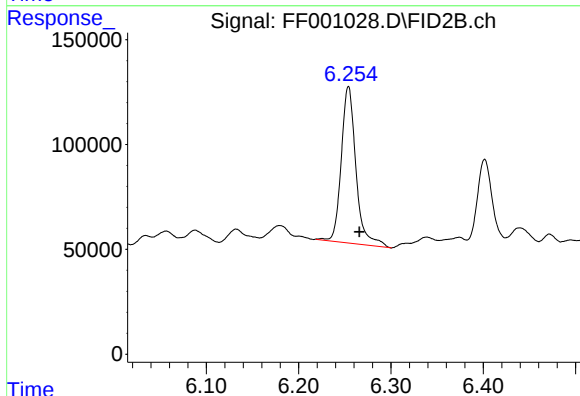


#3 N-DODECANE

R.T.: 6.254 min
Delta R.T.: -0.012 min
Response: 826878
Conc: 5.90 ug/ml

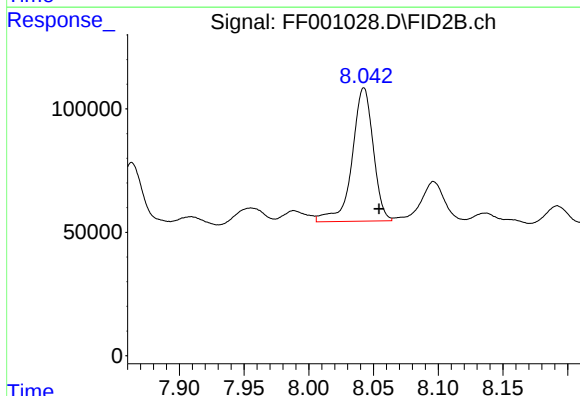


#4 N-TETRADECANE

R.T.: 8.043 min
Delta R.T.: -0.012 min
Response: 614441
Conc: 4.41 ug/ml

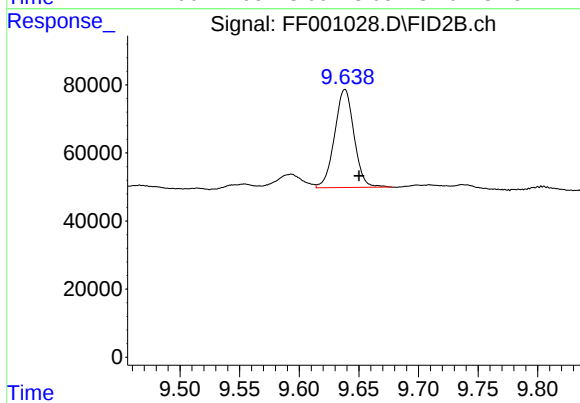

#5 N-HEXADECANE


R.T.: 9.638 min
Delta R.T.: -0.012 min
Response: 327265
Conc: 2.37 ug/ml

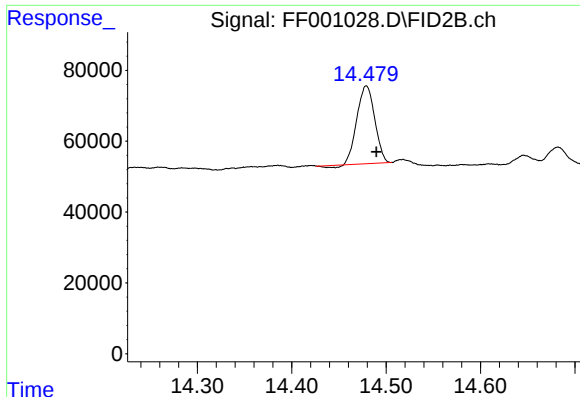

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.479 min
Delta R.T.: -0.011 min
Response: 285760
Conc: 2.48 ug/ml

Instrument :
FID_F
ClientSampleId :

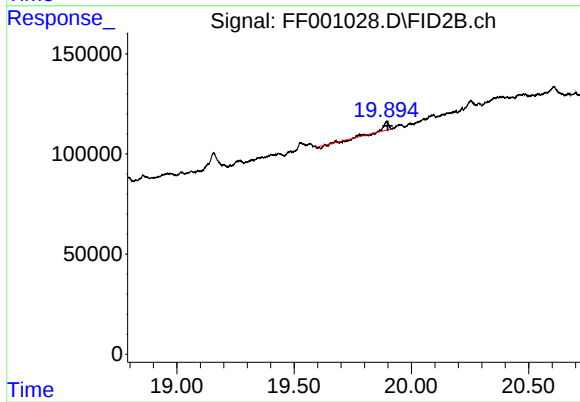

#16 N-HEXATRIACONTANE

R.T.: 19.894 min
Delta R.T.: -0.005 min
Response: 41808
Conc: 0.37 ug/ml