

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001031.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 12:40
 Operator : UA\AJ
 Sample : J3249-01 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:51:10 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.479	205762	1.784 ug/ml
Target Compounds			
4) N-TETRADECANE	8.042	285929	2.054 ug/ml
5) N-HEXADECANE	9.638	368301	2.671 ug/ml
6) N-OCTADECANE	11.076	253946	1.860 ug/ml
7) N-EICOSANE	12.383	349097	2.606 ug/ml
8) N-DOCOSANE	13.592	230684	1.745 ug/ml
10) N-TETRACOSANE	14.647	1252283	9.655 ug/ml
12) N-OCTACOSANE	16.647	363713	2.860 ug/ml
13) N-TRIACONTANE	17.536	228239	1.808 ug/ml
14) N-DOTRIACONTANE	18.368	176893	1.442 ug/ml
15) N-TETRATRIACONTANE	19.162	327009	2.725 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001031.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 12:40
Operator : UA\AJ
Sample : J3249-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:51:10 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

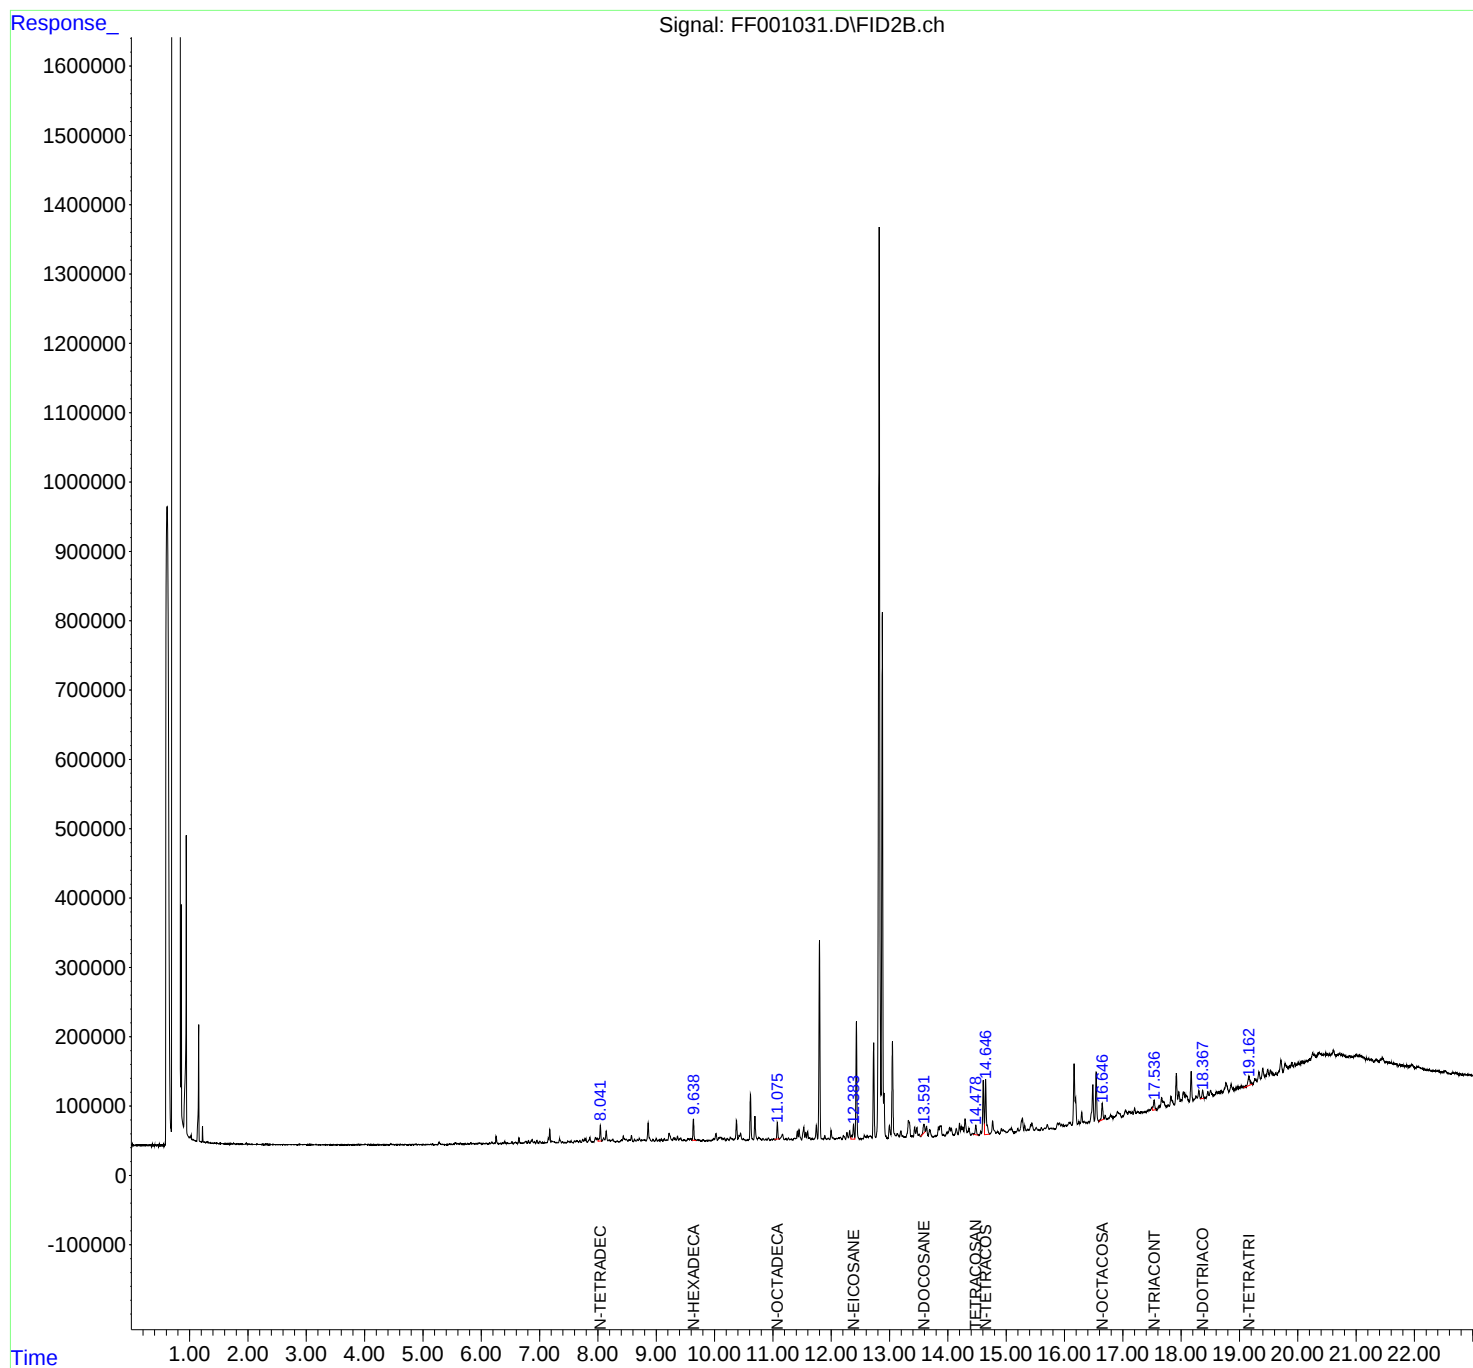


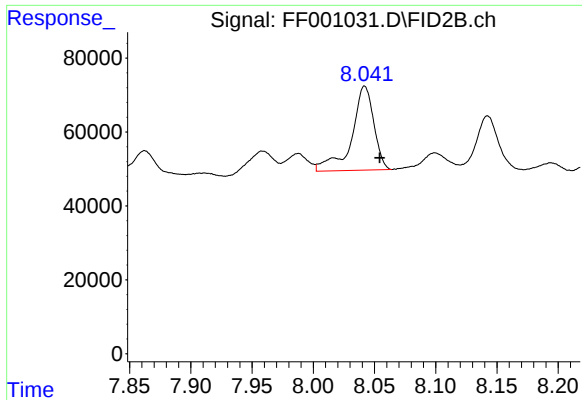

#4 N-TETRADECANE


R.T.: 8.042 min
Delta R.T.: -0.012 min
Response: 285929
Conc: 2.05 ug/ml

Instrument :
FID_F
ClientSampleId :

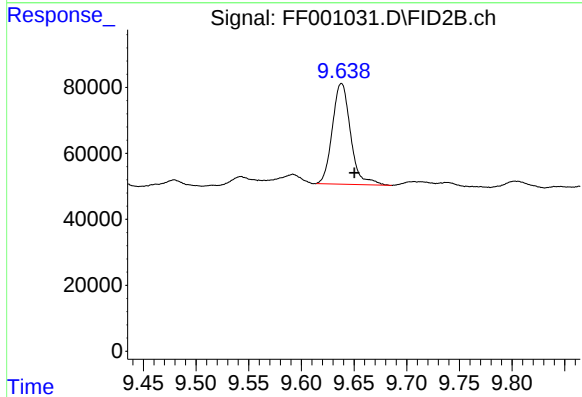


#5 N-HEXADECANE

R.T.: 9.638 min
Delta R.T.: -0.012 min
Response: 368301
Conc: 2.67 ug/ml

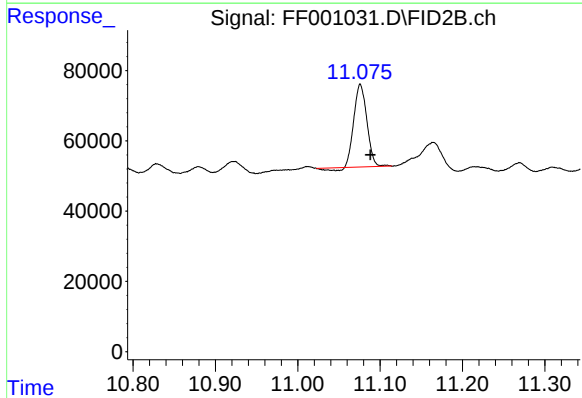


#6 N-OCTADECANE

R.T.: 11.076 min
Delta R.T.: -0.012 min
Response: 253946
Conc: 1.86 ug/ml

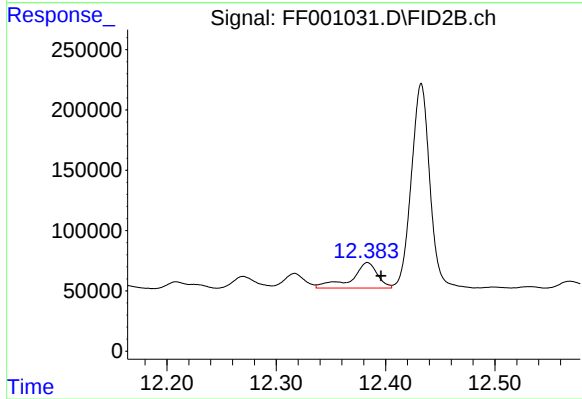

#7 N-EICOSANE


R.T.: 12.383 min
Delta R.T.: -0.012 min
Response: 349097
Conc: 2.61 ug/ml

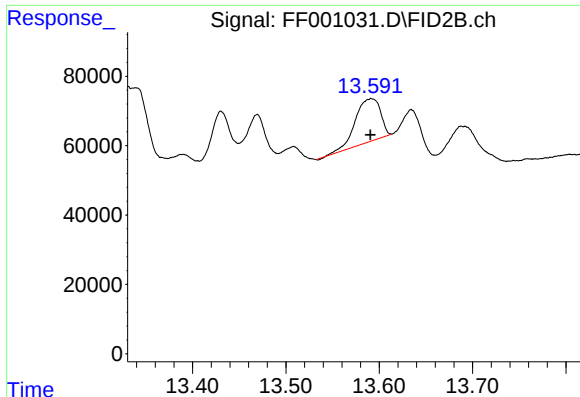

#8 N-DOCOSANE


R.T.: 13.592 min
Delta R.T.: 0.001 min
Response: 230684
Conc: 1.74 ug/ml

Instrument :
FID_F
ClientSampleId :

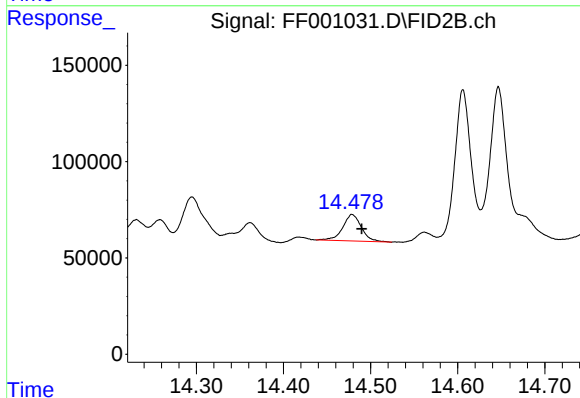


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.479 min
Delta R.T.: -0.011 min
Response: 205762
Conc: 1.78 ug/ml

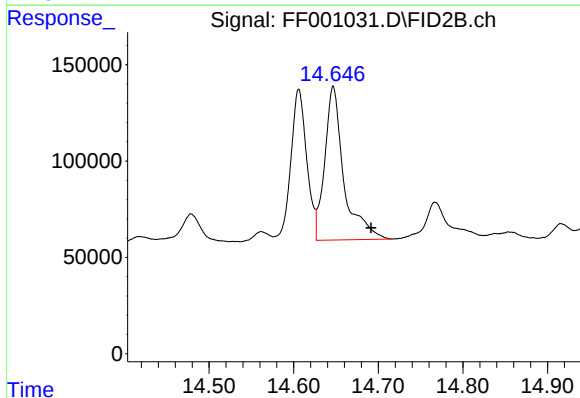


#10 N-TETRACOSANE

R.T.: 14.647 min
Delta R.T.: -0.045 min
Response: 1252283
Conc: 9.65 ug/ml

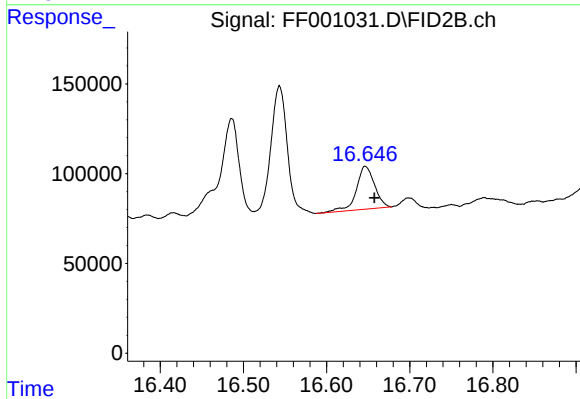

#12 N-OCTACOSANE


R.T.: 16.647 min
Delta R.T.: -0.011 min
Response: 363713
Conc: 2.86 ug/ml

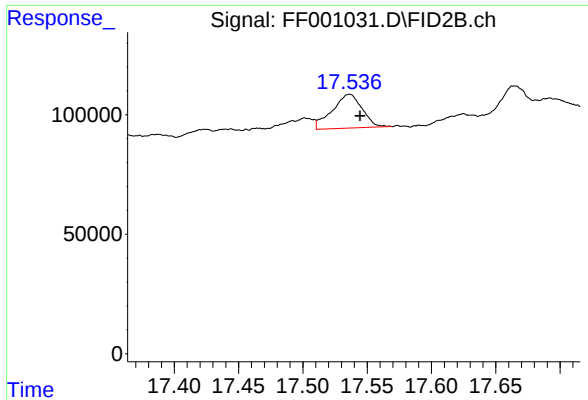

#13 N-TRIACONTANE


R.T.: 17.536 min
Delta R.T.: -0.008 min
Response: 228239
Conc: 1.81 ug/ml

Instrument :
FID_F
ClientSampleId :

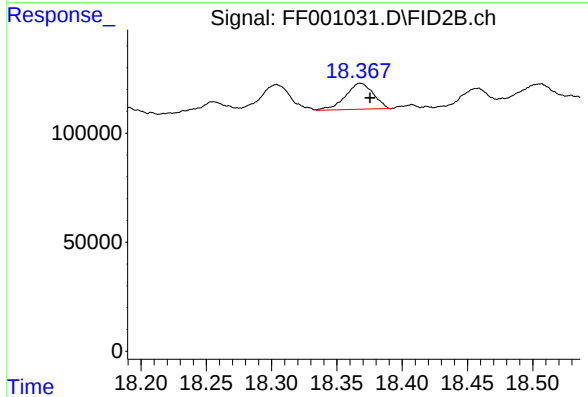

#14 N-DOTRIACONTANE

R.T.: 18.368 min
Delta R.T.: -0.007 min
Response: 176893
Conc: 1.44 ug/ml

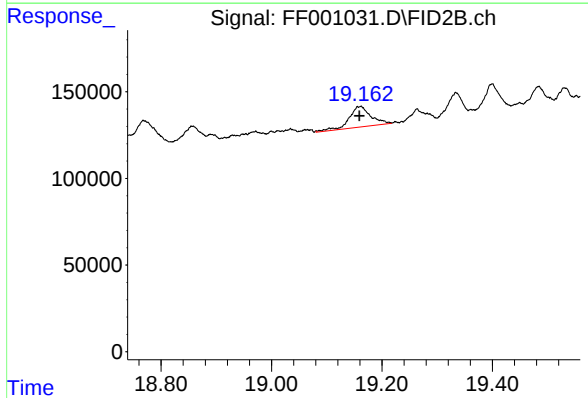

#15 N-TETRATRIACONTANE

R.T.: 19.162 min
Delta R.T.: 0.003 min
Response: 327009
Conc: 2.72 ug/ml