

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001032.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 13:10
 Operator : UA\AJ
 Sample : J3249-03 20X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:51:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.478	325564	2.823 ug/ml
Target Compounds			
7) N-EICOSANE	12.435	4069562	30.375 ug/ml
8) N-DOCOSANE	13.592	422994	3.199 ug/ml
10) N-TETRACOSANE	14.647	1777166	13.701 ug/ml
12) N-OCTACOSANE	16.645	508229	3.997 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001032.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 13:10
Operator : UA\AJ
Sample : J3249-03 20X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:51:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

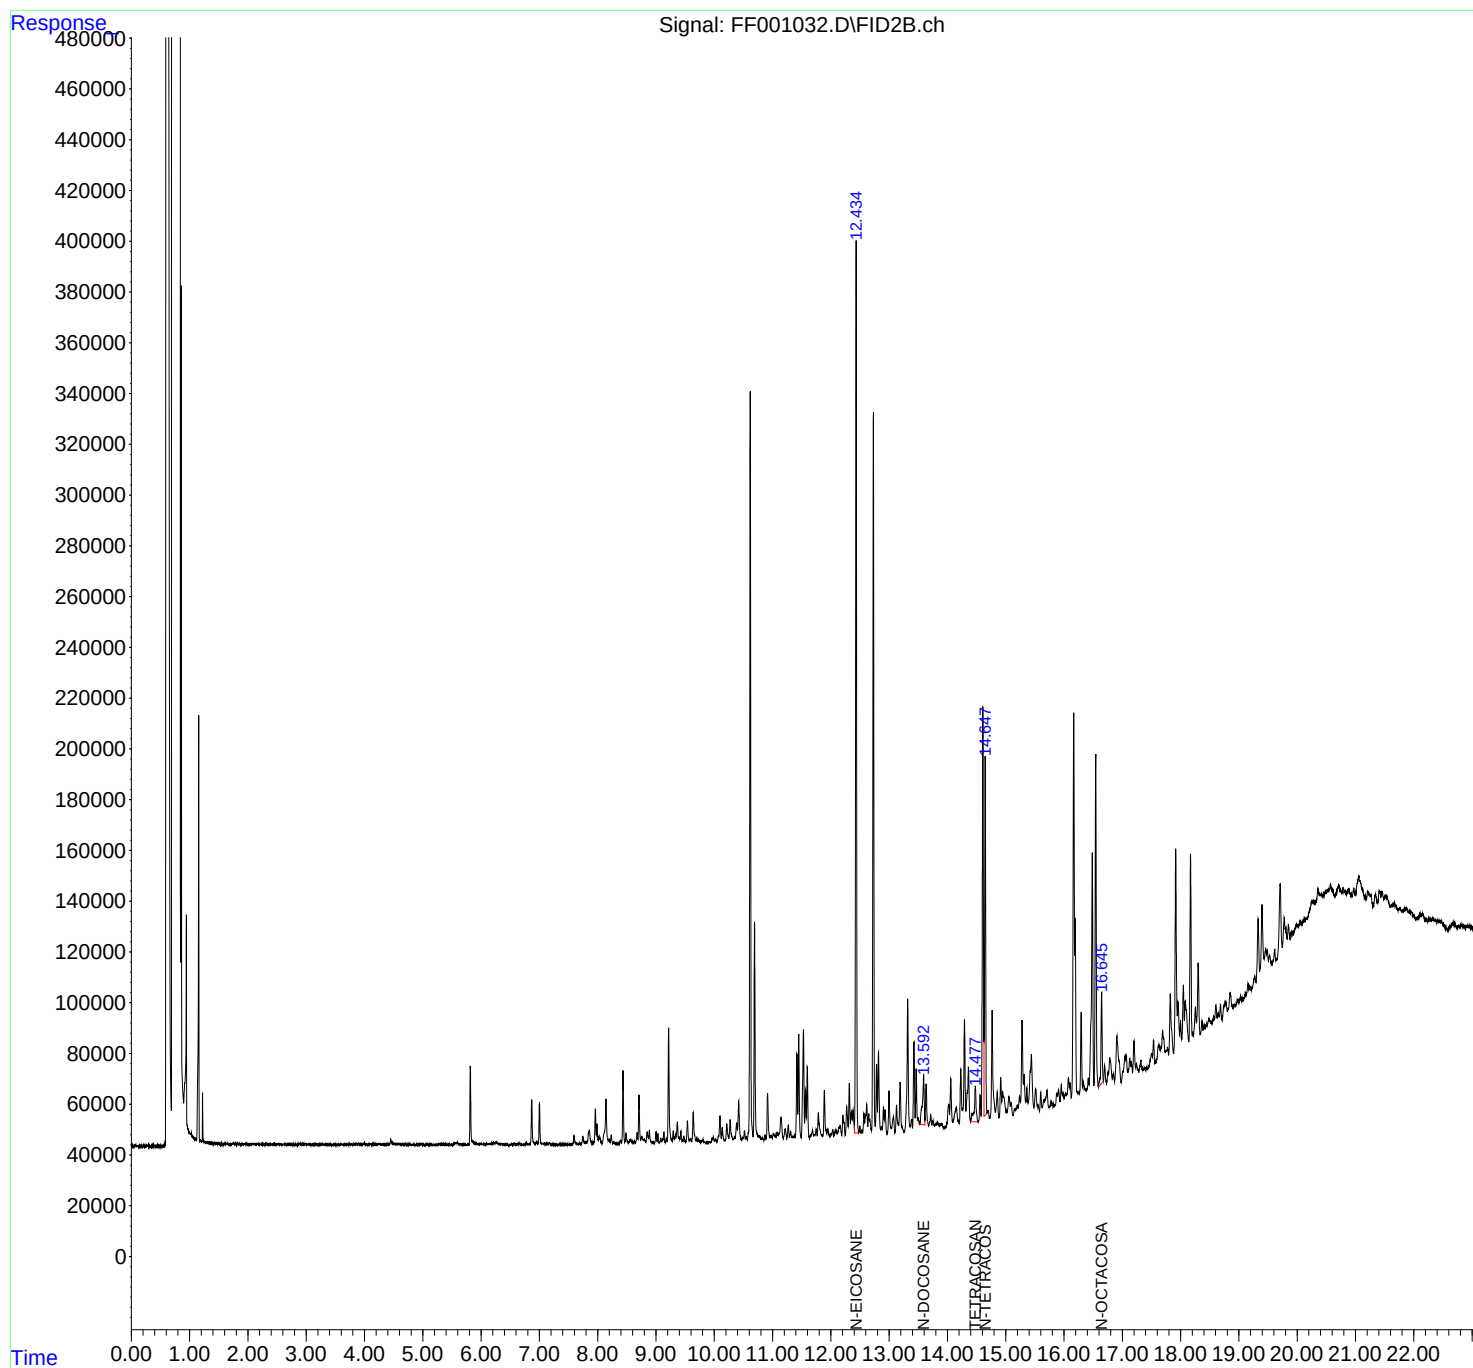


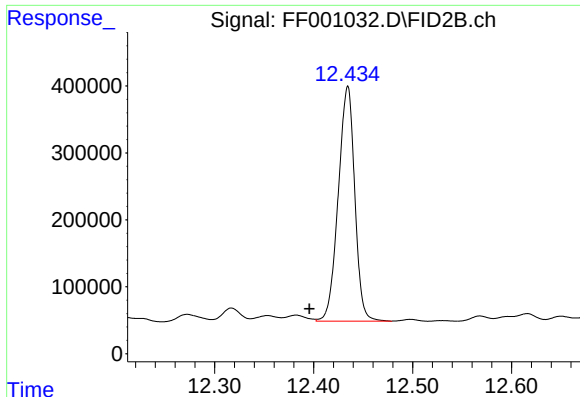

#7 N-EICOSANE


R.T.: 12.435 min
Delta R.T.: 0.039 min
Response: 4069562
Conc: 30.38 ug/ml

Instrument :
FID_F
ClientSampleId :

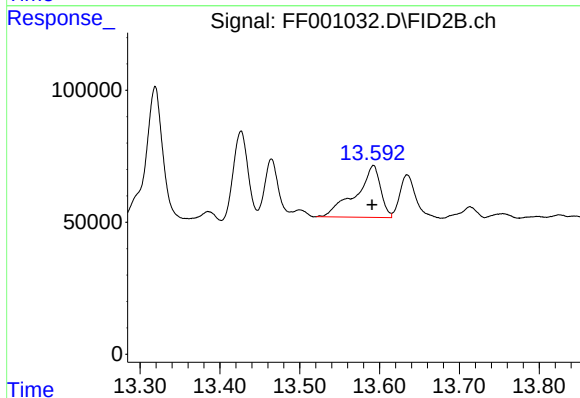


#8 N-DOCOSANE

R.T.: 13.592 min
Delta R.T.: 0.002 min
Response: 422994
Conc: 3.20 ug/ml

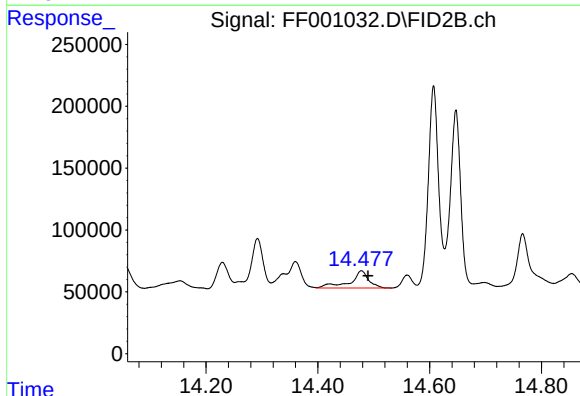


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.478 min
Delta R.T.: -0.012 min
Response: 325564
Conc: 2.82 ug/ml

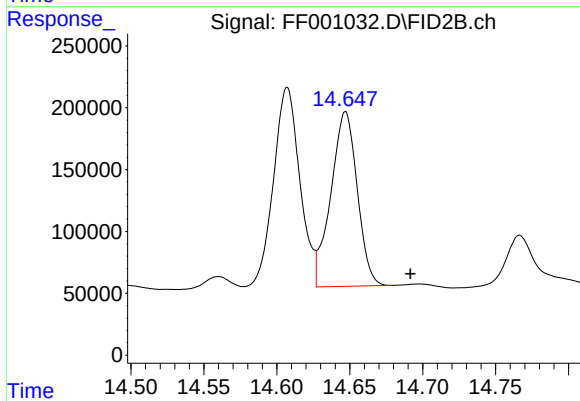

#10 N-TETRACOSANE

R.T.: 14.647 min
Delta R.T.: -0.045 min
Response: 1777166
Conc: 13.70 ug/ml

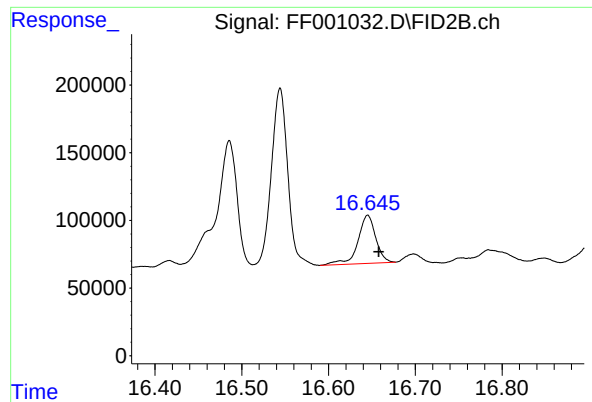

#12 N-OCTACOSANE

R.T.: 16.645 min
Delta R.T.: -0.013 min
Response: 508229
Conc: 4.00 ug/ml

Instrument :
FID_F
ClientSampleId :