

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001033.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 13:40
 Operator : UA\AJ
 Sample : J3249-05 25X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:51:33 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.480	265410	2.301 ug/ml
Target Compounds			
5) N-HEXADECANE	9.640	221685	1.608 ug/ml
7) N-EICOSANE	12.438	5998554	44.773 ug/ml
8) N-DOCOSANE	13.594	645058	4.878 ug/ml
10) N-TETRACOSANE	14.651	2694934	20.777 ug/ml
12) N-OCTACOSANE	16.648	832019	6.543 ug/ml
13) N-TRIACONTANE	17.538	200951	1.591 ug/ml
14) N-DOTRIACONTANE	18.306f	671654	5.476 ug/ml
16) N-HEXATRIACONTANE	19.855	133950	1.173 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001033.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 13:40
Operator : UA\AJ
Sample : J3249-05 25X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:51:33 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

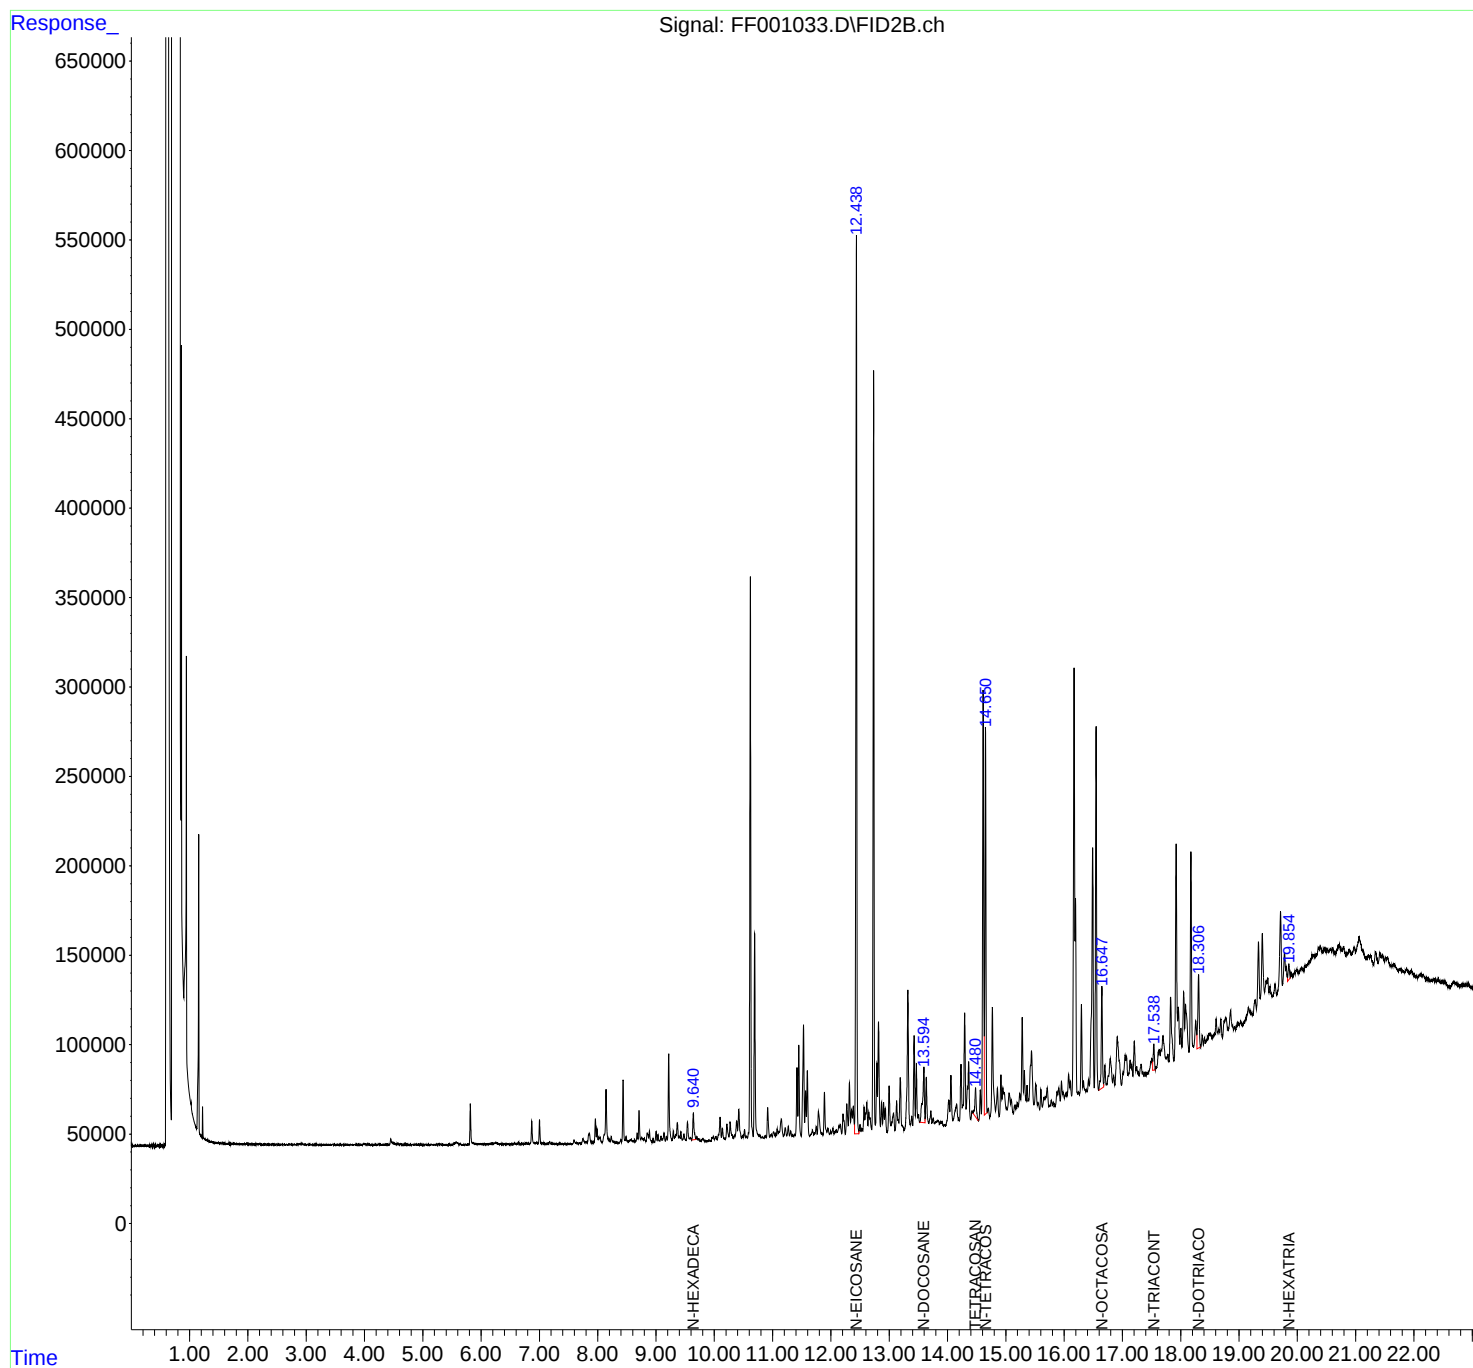


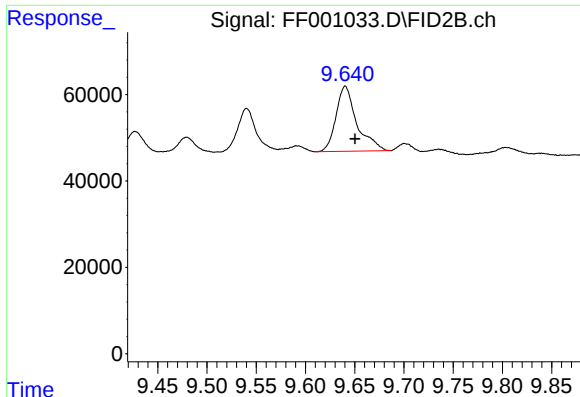

#5 N-HEXADECANE


R.T.: 9.640 min
Delta R.T.: -0.010 min
Response: 221685
Conc: 1.61 ug/ml

Instrument :
FID_F
ClientSampleId :

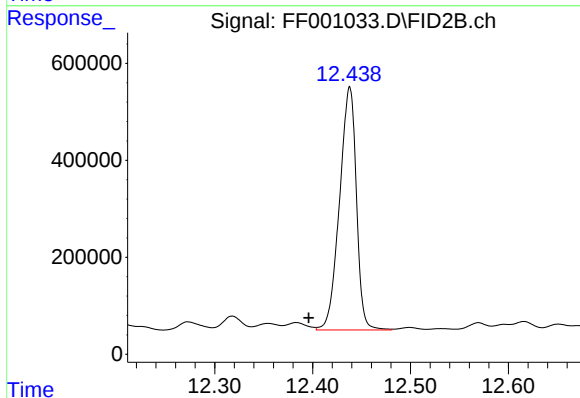


#7 N-EICOSANE

R.T.: 12.438 min
Delta R.T.: 0.042 min
Response: 599854
Conc: 44.77 ug/ml

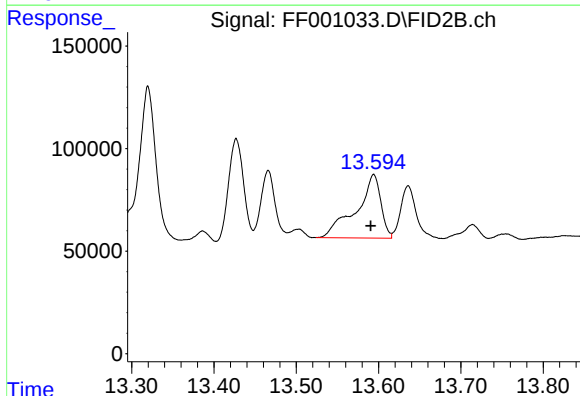


#8 N-DOCOSANE

R.T.: 13.594 min
Delta R.T.: 0.004 min
Response: 645058
Conc: 4.88 ug/ml

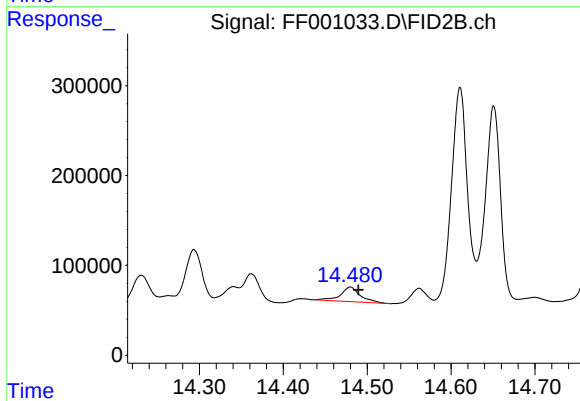

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.480 min
Delta R.T.: -0.010 min
Response: 265410
Conc: 2.30 ug/ml

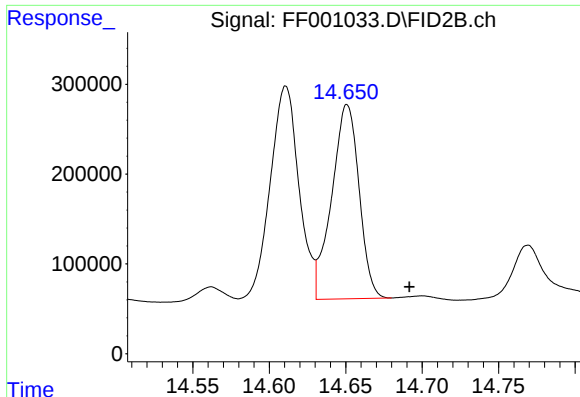

#10 N-TETRACOSANE


R.T.: 14.651 min
Delta R.T.: -0.041 min
Response: 2694934
Conc: 20.78 ug/ml

Instrument :
FID_F
ClientSampleId :

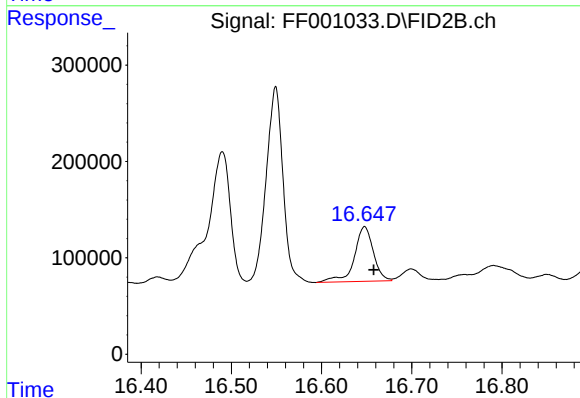


#12 N-OCTACOSANE

R.T.: 16.648 min
Delta R.T.: -0.010 min
Response: 832019
Conc: 6.54 ug/ml

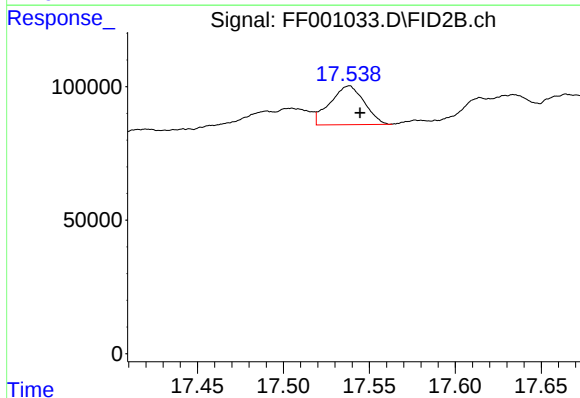


#13 N-TRIACONTANE

R.T.: 17.538 min
Delta R.T.: -0.006 min
Response: 200951
Conc: 1.59 ug/ml

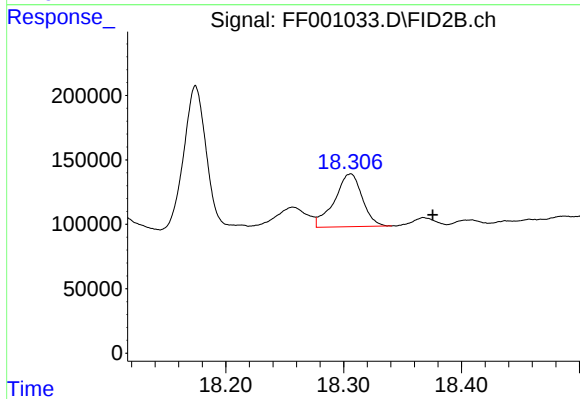

#14 N-DOTRIACONTANE

R.T.: 18.306 min
Delta R.T.: -0.070 min
Response: 671654
Conc: 5.48 ug/ml

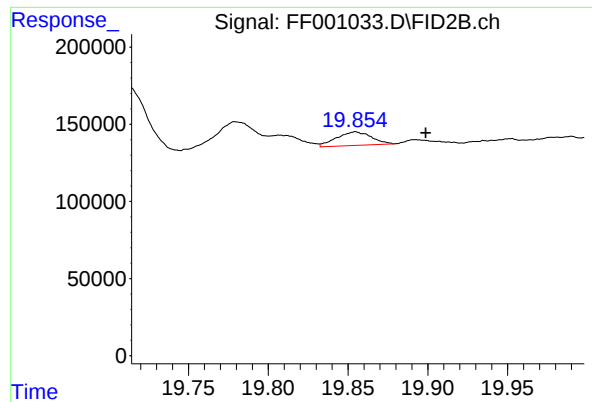

#16 N-HEXATRIACONTANE

R.T.: 19.855 min
Delta R.T.: -0.044 min
Response: 133950
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :