

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001034.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 14:11
 Operator : UA\AJ
 Sample : J3249-07 25X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:51:44 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
5) N-HEXADECANE	9.639	231275	1.677 ug/ml
6) N-OCTADECANE	11.076	151764	1.111 ug/ml
7) N-EICOSANE	12.383	212013	1.582 ug/ml
8) N-DOCOSANE	13.592	156564	1.184 ug/ml
10) N-TETRACOSANE	14.648	1318829	10.168 ug/ml
12) N-OCTACOSANE	16.645	316909	2.492 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001034.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 14:11
Operator : UA\AJ
Sample : J3249-07 25X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:51:44 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

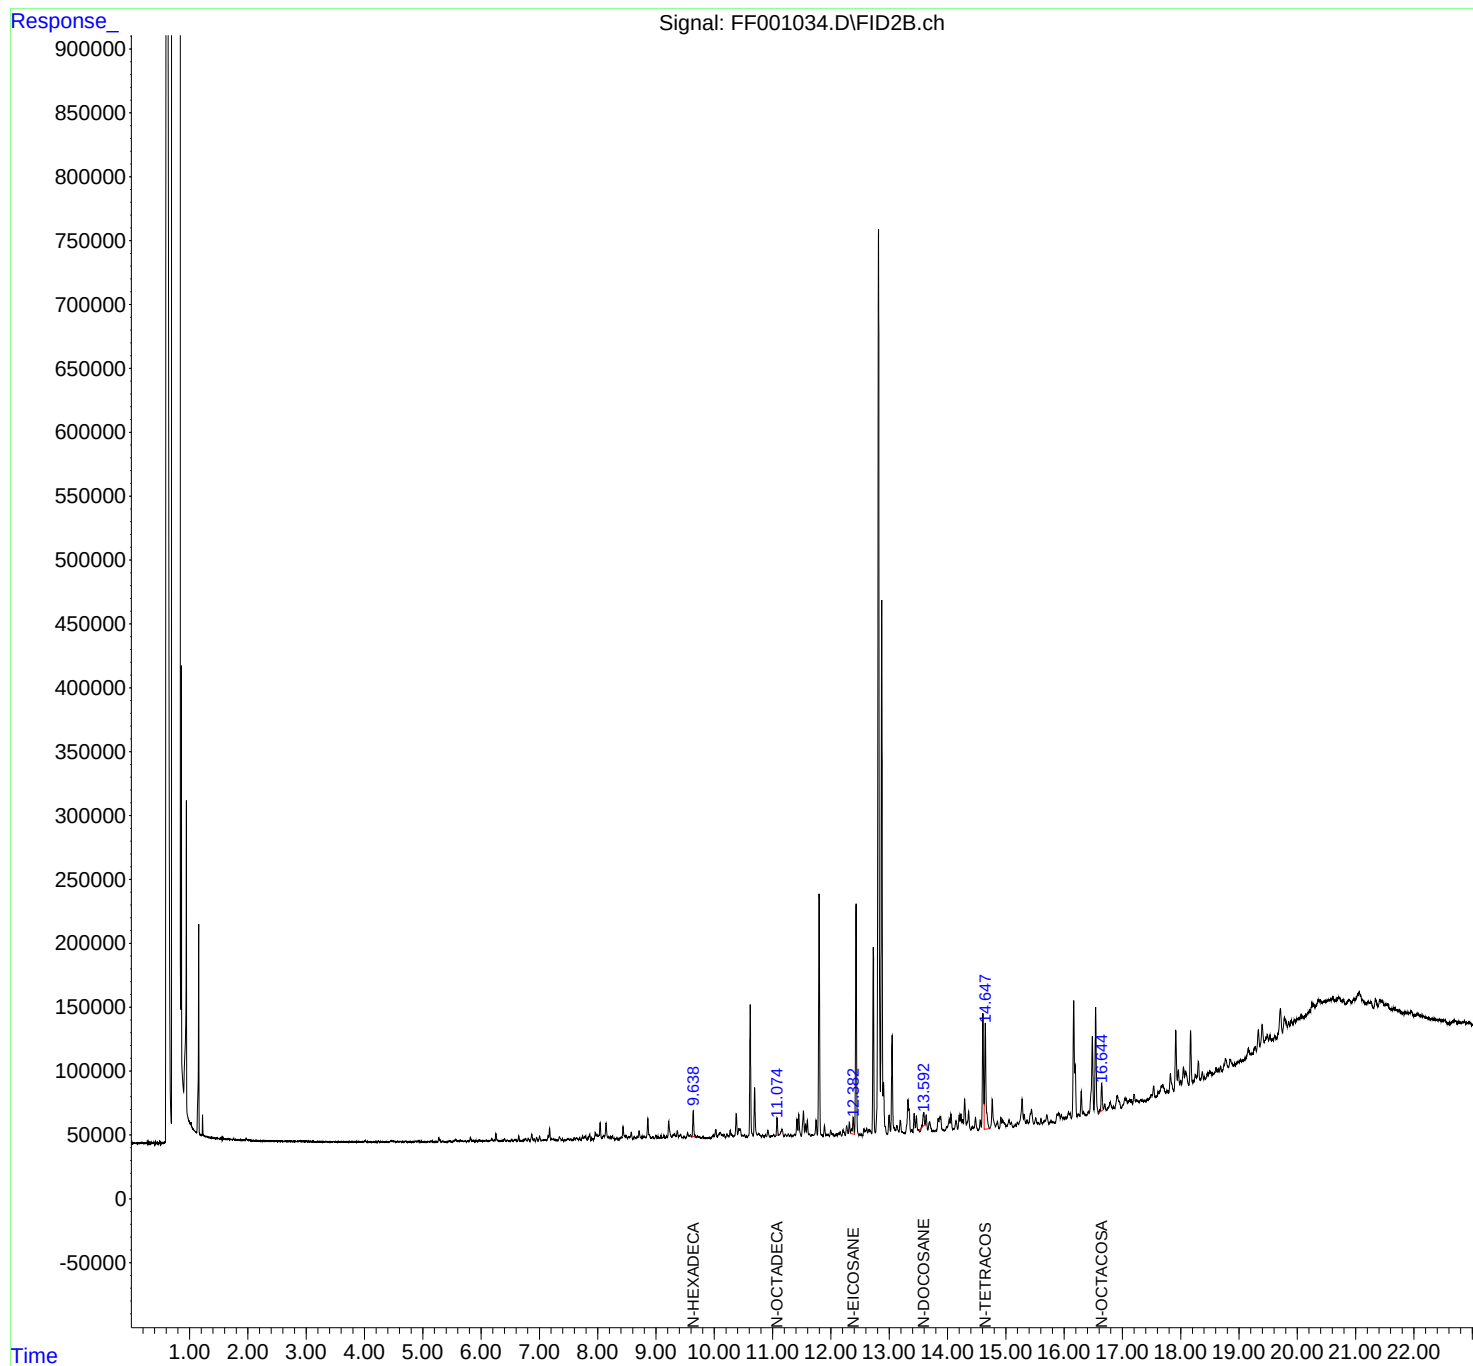


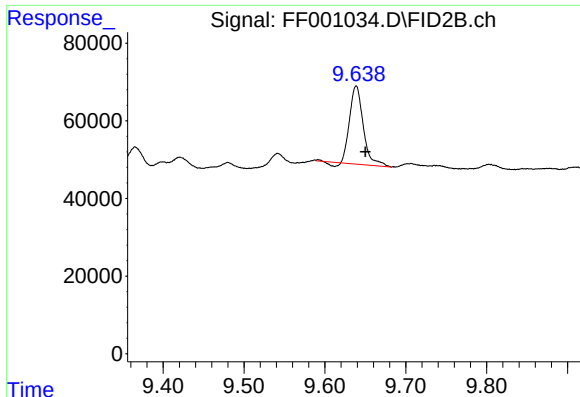

#5 N-HEXADECANE


R.T.: 9.639 min
Delta R.T.: -0.012 min
Response: 231275
Conc: 1.68 ug/ml

Instrument :
FID_F
ClientSampleId :

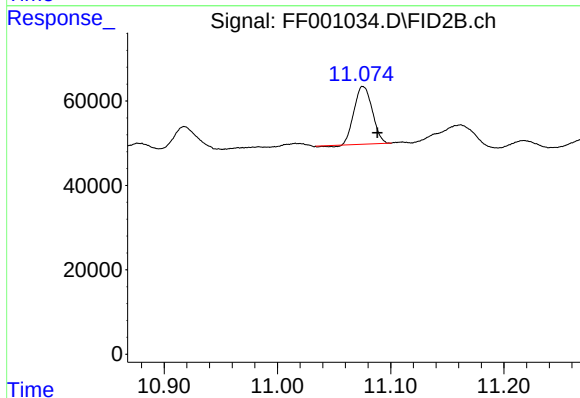


#6 N-OCTADECANE

R.T.: 11.076 min
Delta R.T.: -0.013 min
Response: 151764
Conc: 1.11 ug/ml

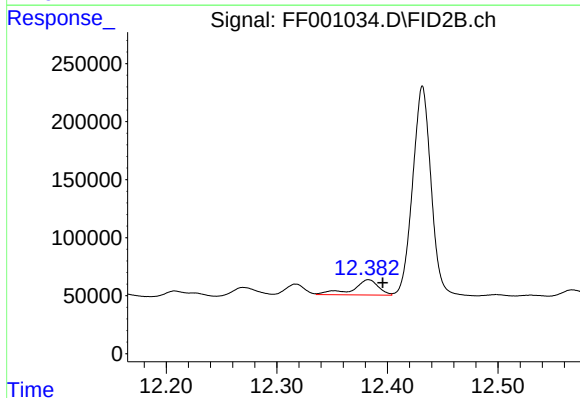


#7 N-EICOSANE

R.T.: 12.383 min
Delta R.T.: -0.013 min
Response: 212013
Conc: 1.58 ug/ml

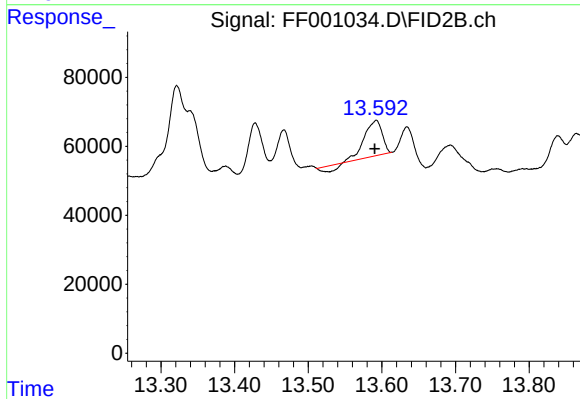

#8 N-DOCOSANE


R.T.: 13.592 min
Delta R.T.: 0.002 min
Response: 156564
Conc: 1.18 ug/ml

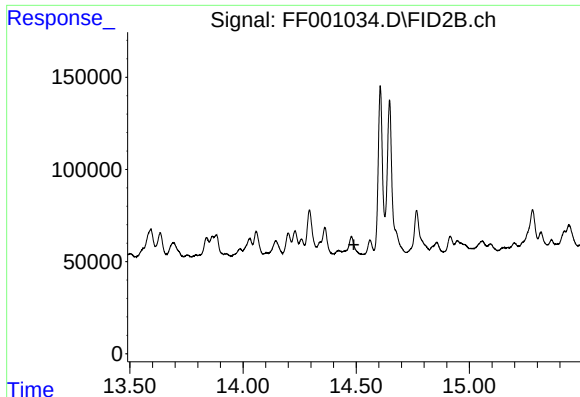

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.490 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

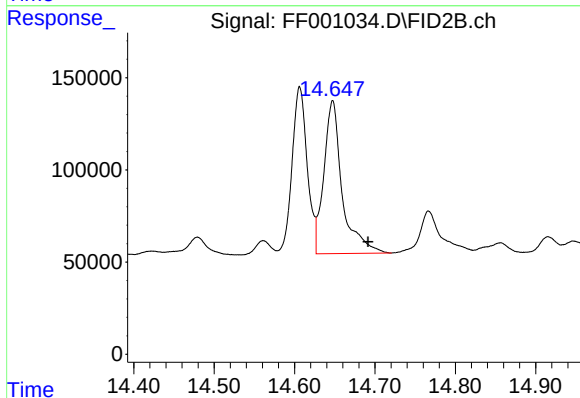

#10 N-TETRACOSANE

R.T.: 14.648 min
Delta R.T.: -0.044 min
Response: 1318829
Conc: 10.17 ug/ml

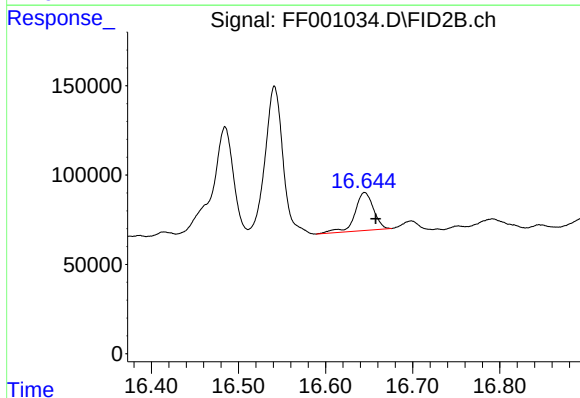

#12 N-OCTACOSANE

R.T.: 16.645 min
Delta R.T.: -0.013 min
Response: 316909
Conc: 2.49 ug/ml