

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001037.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 15:42
Operator : UA\AJ
Sample : J3245-13 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:52:15 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.431	553225	4.129 ug/ml
10)	N-TETRACOSANE	14.647	371681	2.865 ug/ml
12)	N-OCTACOSANE	16.654	290443	2.284 ug/ml
13)	N-TRIACONTANE	17.530	369758	2.928 ug/ml
15)	N-TETRATRIACONTANE	19.165	350775	2.923 ug/ml
16)	N-HEXATRIACONTANE	19.953f	113405	0.993 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001037.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 15:42
Operator : UA\AJ
Sample : J3245-13 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:52:15 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

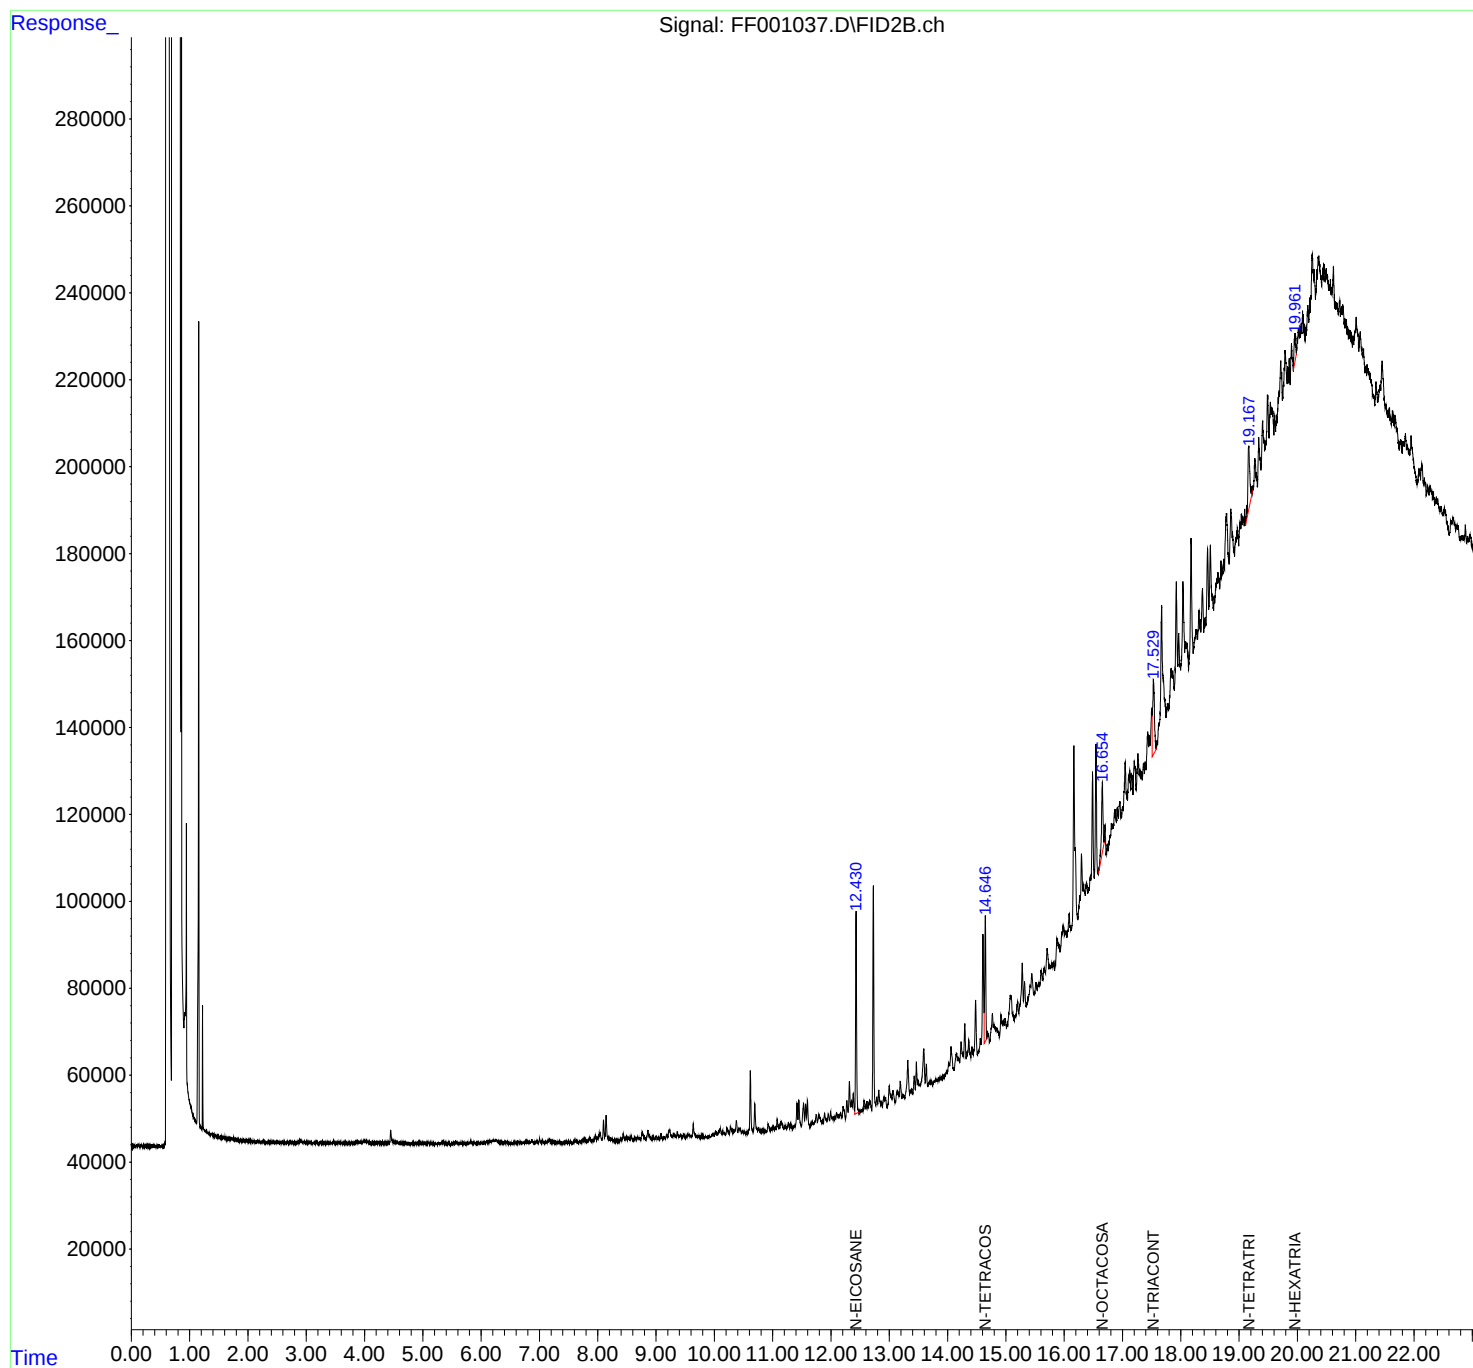


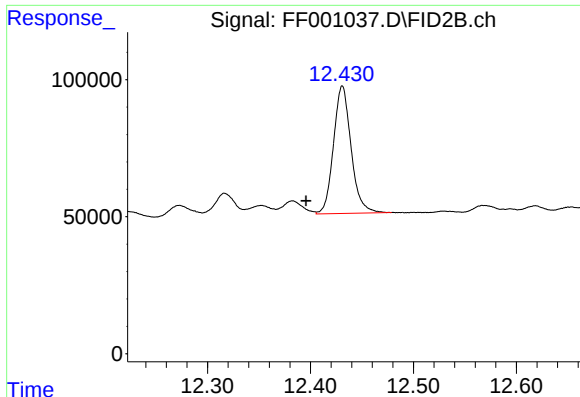

#7 N-EICOSANE


R.T.: 12.431 min
Delta R.T.: 0.035 min
Response: 553225
Conc: 4.13 ug/ml

Instrument :
FID_F
ClientSampleId :

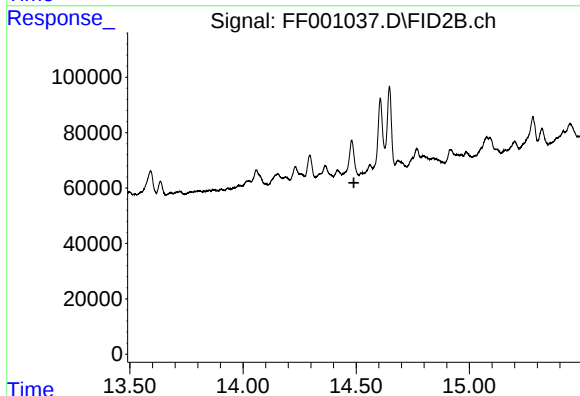


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.490 min
Response: 0
Conc: N.D.

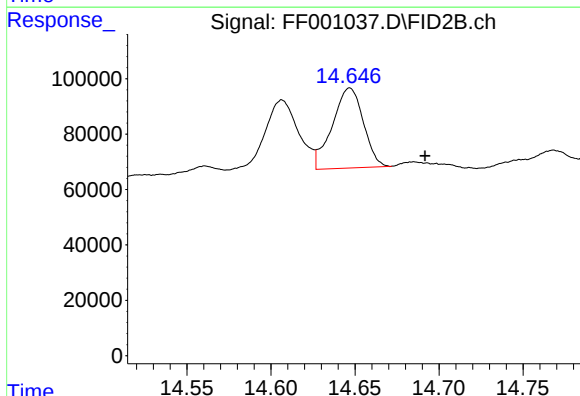


#10 N-TETRACOSANE

R.T.: 14.647 min
Delta R.T.: -0.045 min
Response: 371681
Conc: 2.87 ug/ml

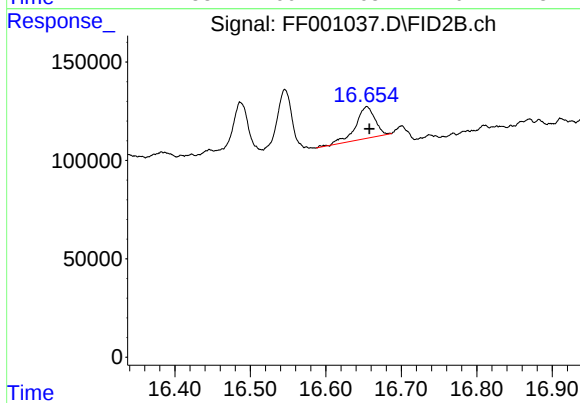

#12 N-OCTACOSANE


R.T.: 16.654 min
Delta R.T.: -0.003 min
Response: 290443
Conc: 2.28 ug/ml

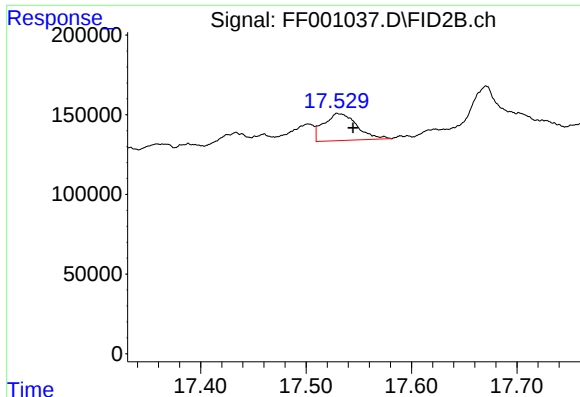

#13 N-TRIACONTANE


R.T.: 17.530 min
Delta R.T.: -0.015 min
Response: 369758
Conc: 2.93 ug/ml

Instrument :
FID_F
ClientSampleId :

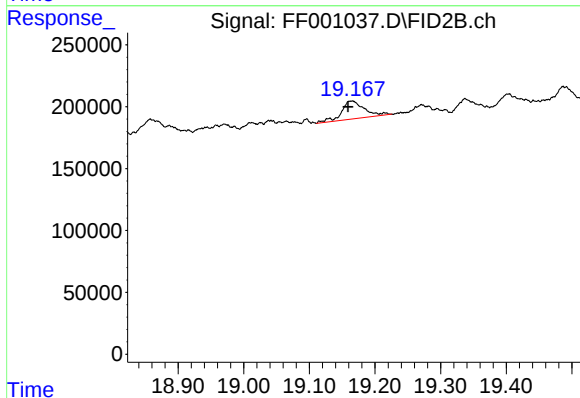

#15 N-TETRATRIACONTANE

R.T.: 19.165 min
Delta R.T.: 0.006 min
Response: 350775
Conc: 2.92 ug/ml

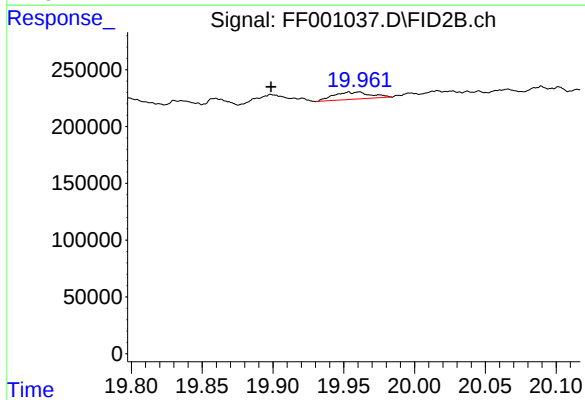

#16 N-HEXATRIACONTANE

R.T.: 19.953 min
Delta R.T.: 0.055 min
Response: 113405
Conc: 0.99 ug/ml