

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001038.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 16:12
 Operator : UA\AJ
 Sample : J3245-15 10X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:52:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.480	194054	1.683 ug/ml
Target Compounds			
7) N-EICOSANE	12.431	335683	2.506 ug/ml
10) N-TETRACOSANE	14.647	232255	1.791 ug/ml
12) N-OCTACOSANE	16.656	232700	1.830 ug/ml
15) N-TETRATRIACONTANE	19.167	392603	3.271 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001038.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 16:12
Operator : UA\AJ
Sample : J3245-15 10X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:52:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

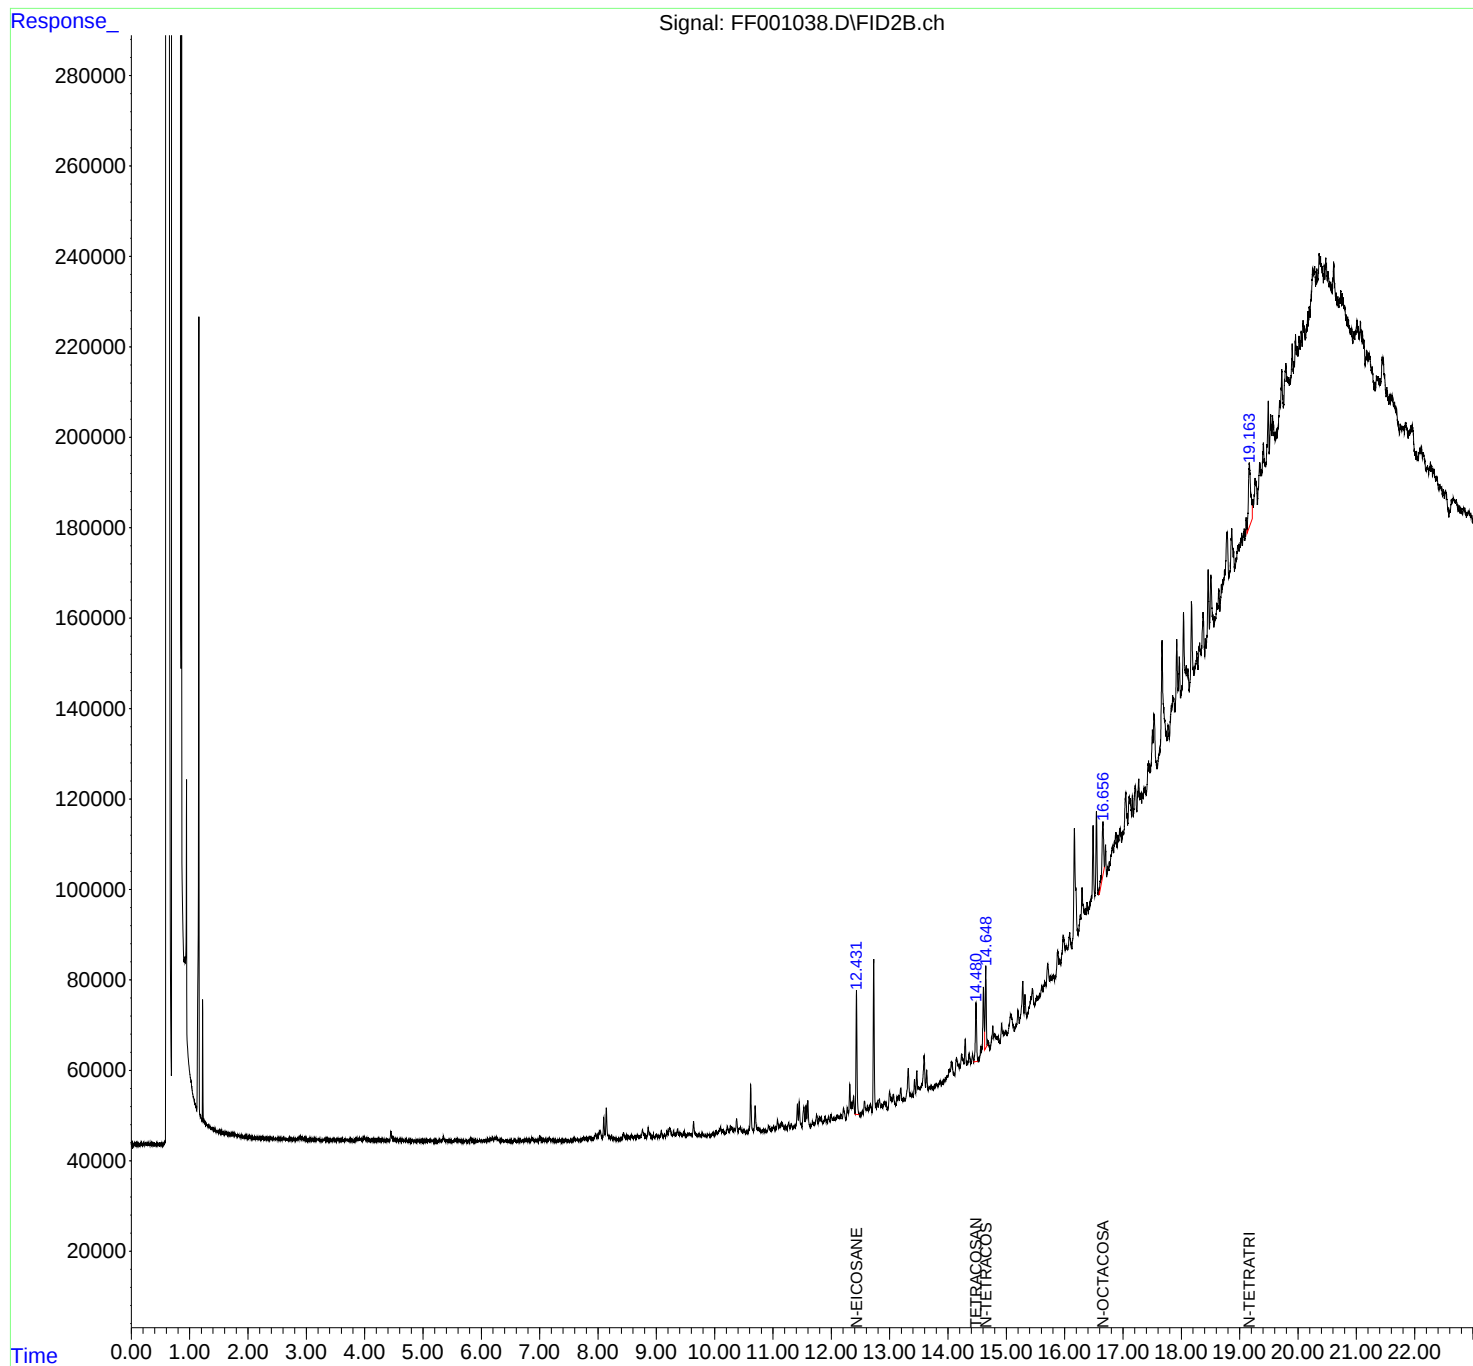


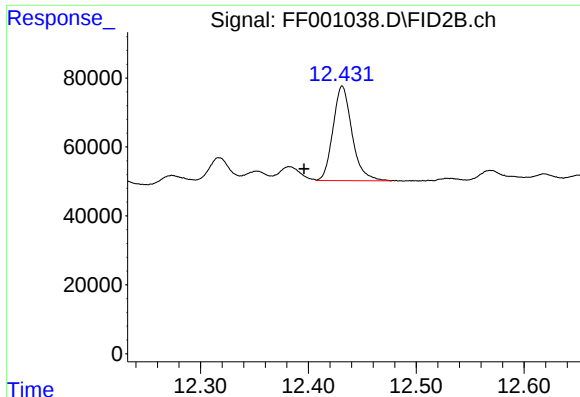

#7 N-EICOSANE


R.T.: 12.431 min
Delta R.T.: 0.036 min
Response: 335683
Conc: 2.51 ug/ml

Instrument :
FID_F
ClientSampleId :

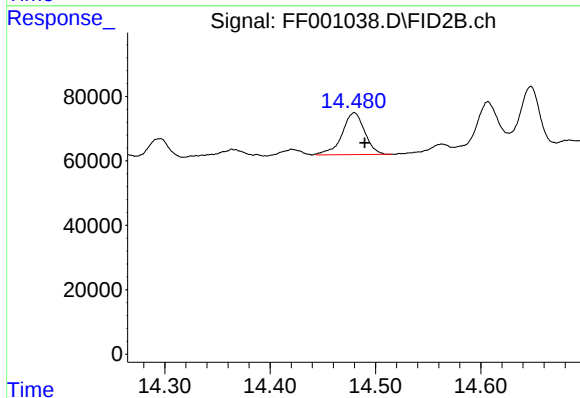


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.480 min
Delta R.T.: -0.010 min
Response: 194054
Conc: 1.68 ug/ml

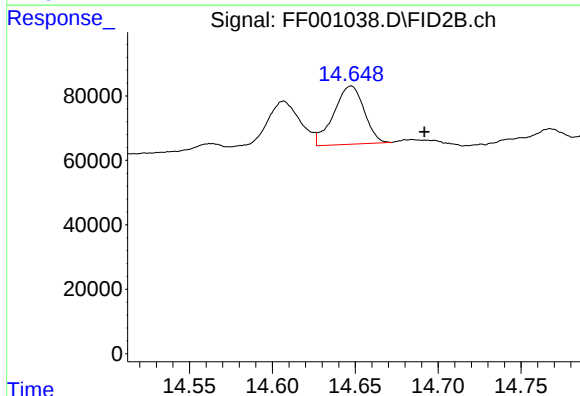


#10 N-TETRACOSANE

R.T.: 14.647 min
Delta R.T.: -0.044 min
Response: 232255
Conc: 1.79 ug/ml

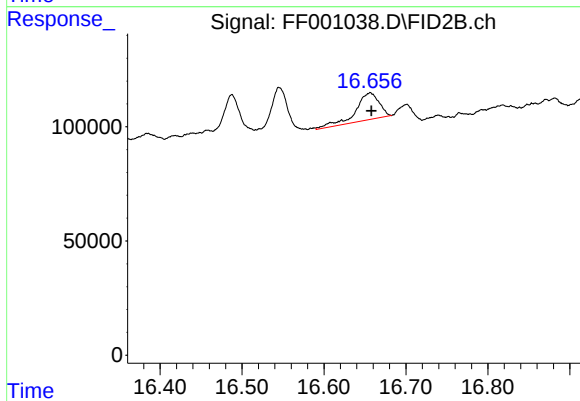

#12 N-OCTACOSANE

R.T.: 16.656 min
Delta R.T.: -0.001 min
Response: 232700
Conc: 1.83 ug/ml

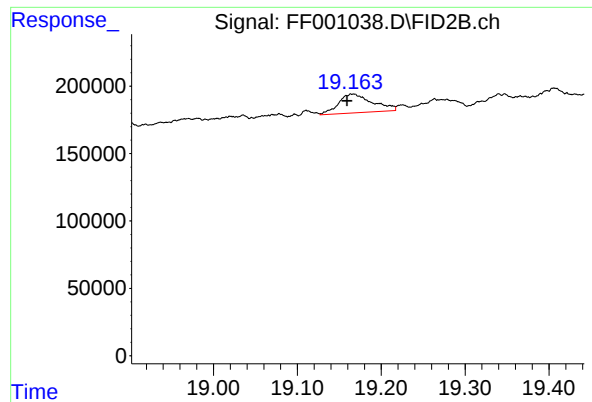

#15 N-TETRATRIACONTANE

R.T.: 19.167 min

Delta R.T.: 0.007 min

Response: 392603

Conc: 3.27 ug/ml

Instrument :
FID_F
ClientSampleId :