

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062018\  
 Data File : FF001039.D  
 Signal(s) : FID2B.ch  
 Acq On : 20 Jun 2018 16:42  
 Operator : UA\AJ  
 Sample : J3247-05 10X  
 Misc :  
 ALS Vial : 66 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jun 21 07:52:37 2018  
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF060118.M  
 Quant Title :  
 QLast Update : Fri Jun 01 16:01:51 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units  |
|-------------------------------|--------|----------|-------------|
| -----                         |        |          |             |
| System Monitoring Compounds   |        |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.480 | 224539   | 1.947 ug/ml |
| Target Compounds              |        |          |             |
| 7) N-EICOSANE                 | 12.432 | 516552   | 3.856 ug/ml |
| 10) N-TETRACOSANE             | 14.647 | 218639   | 1.686 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.158 | 214932   | 1.791 ug/ml |
| 16) N-HEXATRIACONTANE         | 19.897 | 148779   | 1.303 ug/ml |
| -----                         |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062018\  
Data File : FF001039.D  
Signal(s) : FID2B.ch  
Acq On : 20 Jun 2018 16:42  
Operator : UA\AJ  
Sample : J3247-05 10X  
Misc :  
ALS Vial : 66 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 21 07:52:37 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF060118.M  
Quant Title :  
QLast Update : Fri Jun 01 16:01:51 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

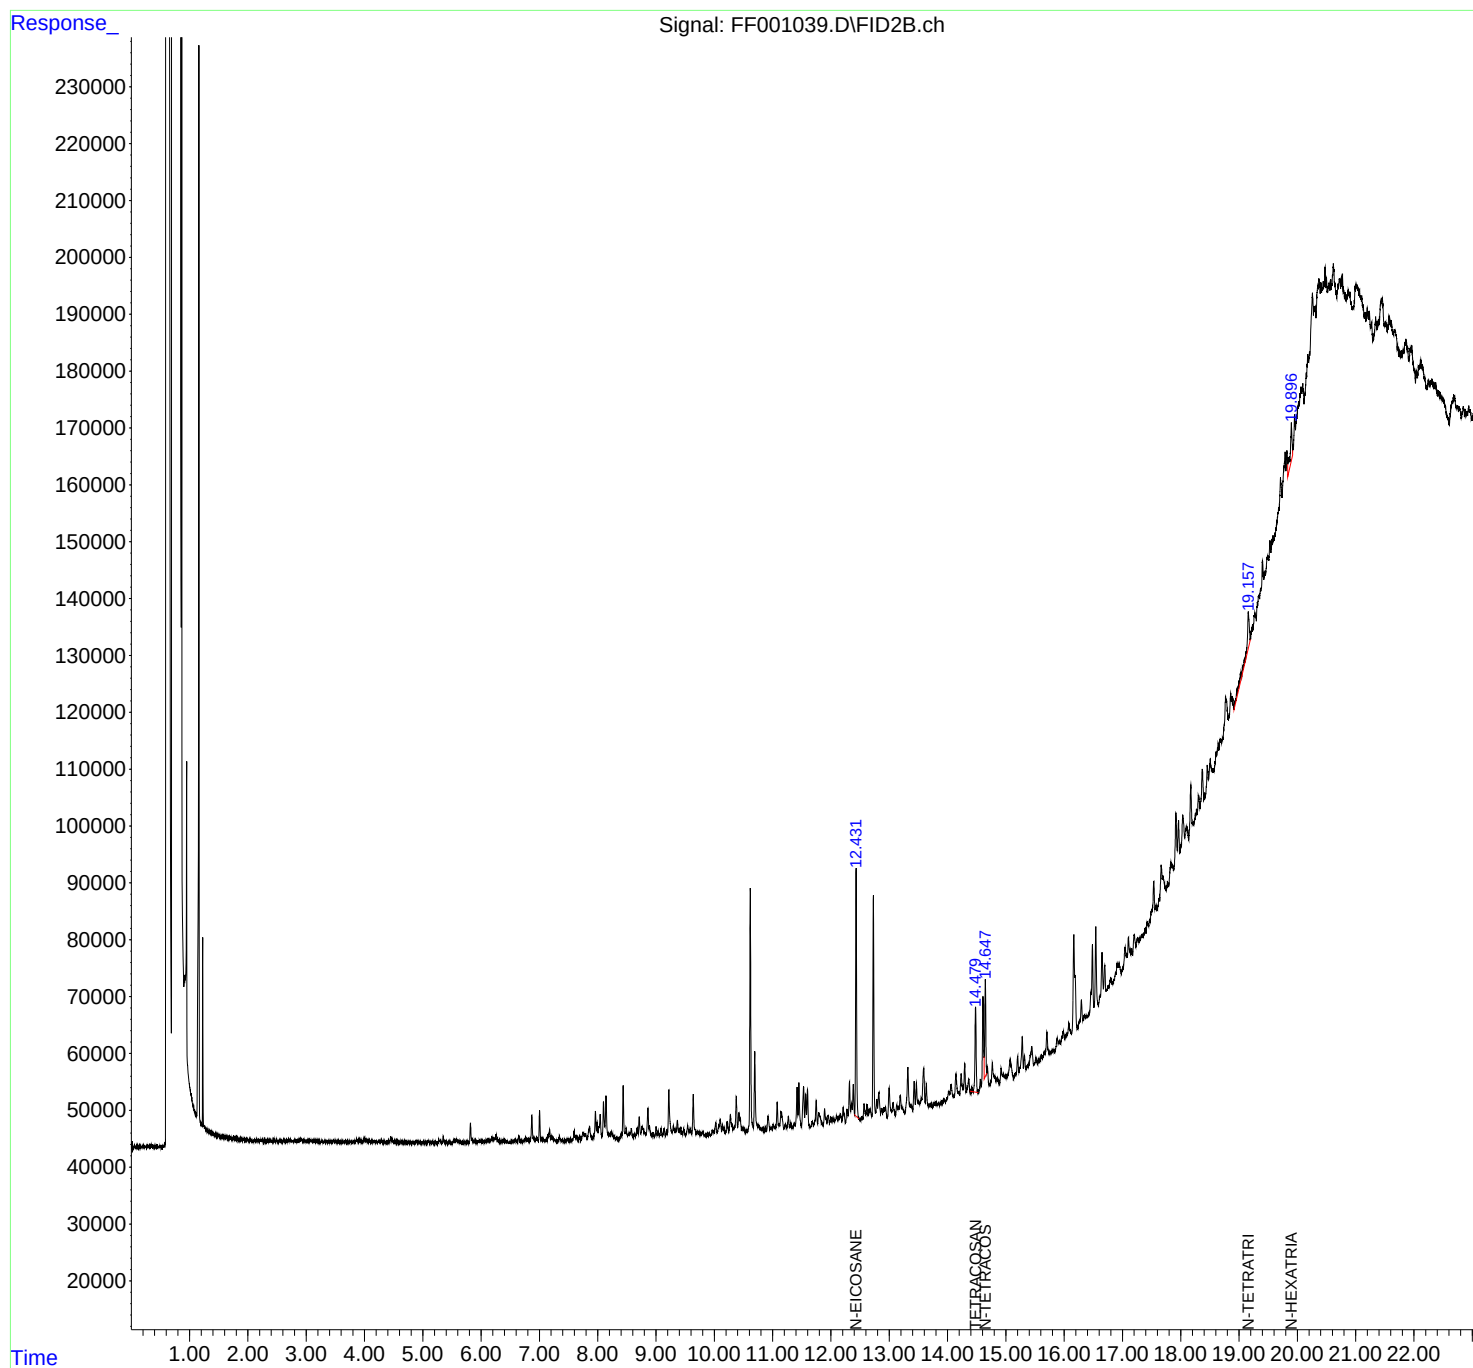


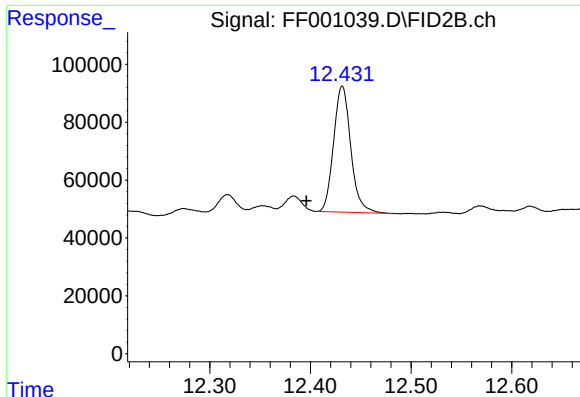

#7 N-EICOSANE


R.T.: 12.432 min  
Delta R.T.: 0.036 min  
Response: 516552  
Conc: 3.86 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

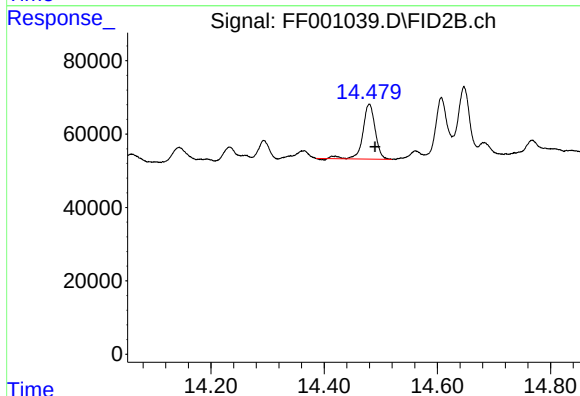


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.480 min  
Delta R.T.: -0.010 min  
Response: 224539  
Conc: 1.95 ug/ml

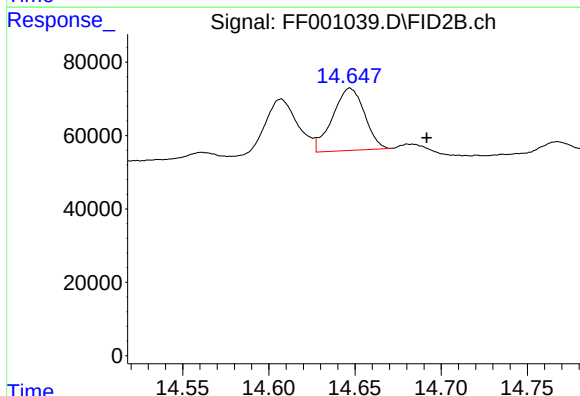


#10 N-TETRACOSANE

R.T.: 14.647 min  
Delta R.T.: -0.044 min  
Response: 218639  
Conc: 1.69 ug/ml

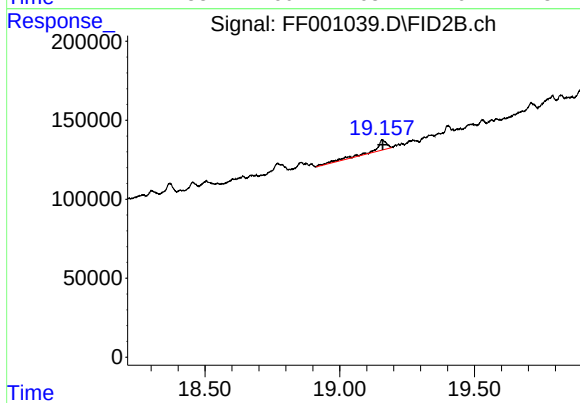

#15 N-TETRATRIACONTANE

R.T.: 19.158 min  
Delta R.T.: -0.001 min  
Response: 214932  
Conc: 1.79 ug/ml

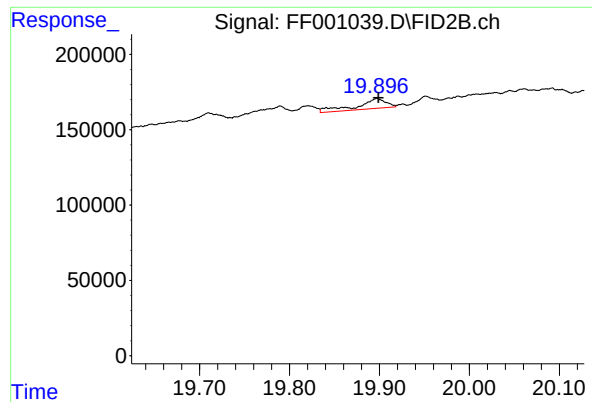

#16 N-HEXATRIACONTANE

R.T.: 19.897 min  
Delta R.T.: -0.002 min  
Response: 148779  
Conc: 1.30 ug/ml

Instrument :  
FID\_F  
ClientSampleId :