

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001040.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 17:13
 Operator : UA\AJ
 Sample : J3245-09MS 10X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:52:48 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.481	218985	1.899 ug/ml
Target Compounds			
1) N-OCTANE	2.160	139583	0.991 ug/ml
2) N-DECANE	4.240	209247	1.493 ug/ml
3) N-DODECANE	6.253	210659	1.503 ug/ml
4) N-TETRADECANE	8.042	235962	1.695 ug/ml
5) N-HEXADECANE	9.638	246944	1.791 ug/ml
6) N-OCTADECANE	11.077	222212	1.627 ug/ml
7) N-EICOSANE	12.385	280507	2.094 ug/ml
8) N-DOCOSANE	13.582	333742	2.524 ug/ml
10) N-TETRACOSANE	14.684	234517	1.808 ug/ml
11) N-HEXACOSANE	15.704	278731	2.170 ug/ml
12) N-OCTACOSANE	16.654	512866	4.033 ug/ml
13) N-TRIACONTANE	17.538	597320	4.730 ug/ml
14) N-DOTRIACONTANE	18.373	316902	2.584 ug/ml
15) N-TETRATRIACONTANE	19.161	415562	3.463 ug/ml
16) N-HEXATRIACONTANE	19.901	226669	1.985 ug/ml
17) N-OCTATRIACONTANE	20.616	328344	3.191 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001040.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 17:13
Operator : UA\AJ
Sample : J3245-09MS 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:52:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

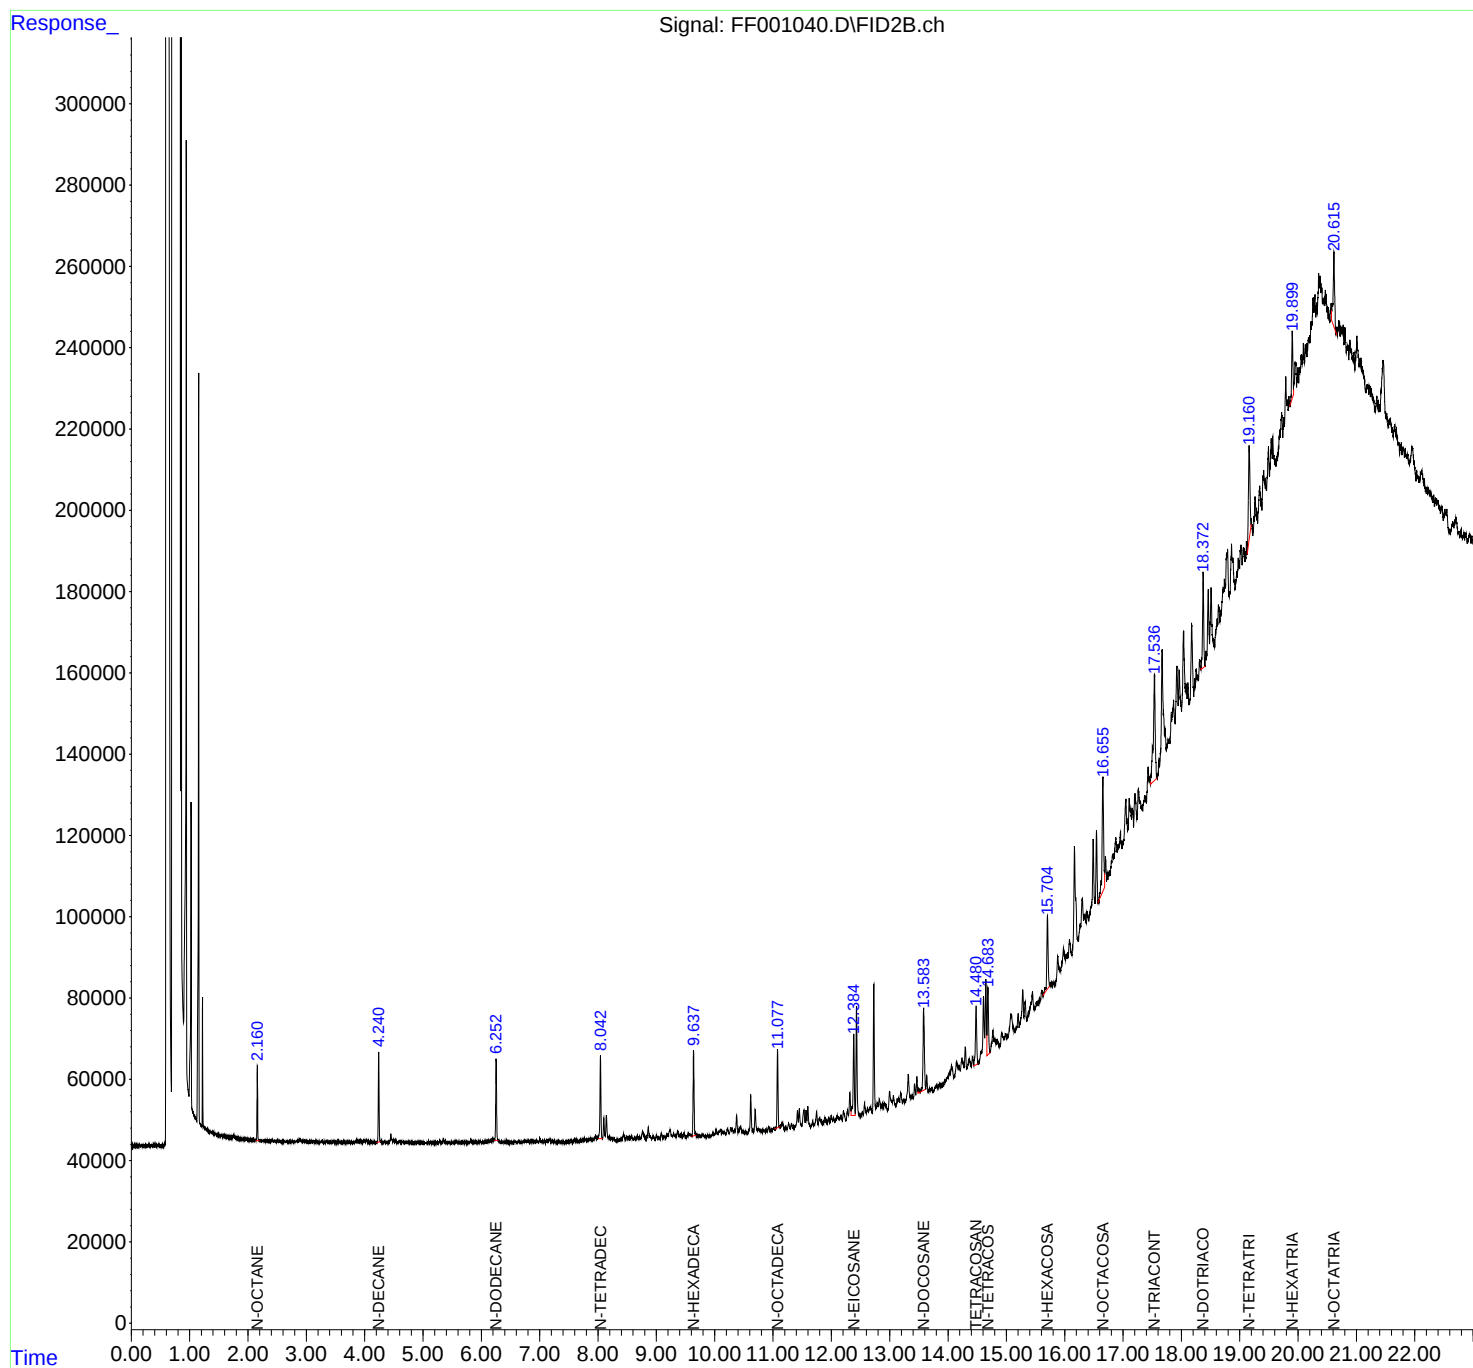


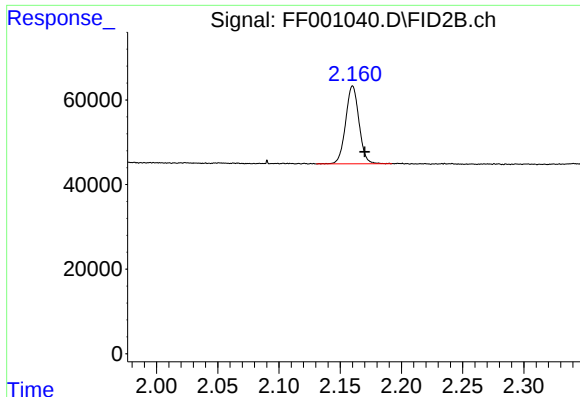

#1 N-OCTANE


R.T.: 2.160 min
Delta R.T.: -0.010 min
Response: 139583
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :

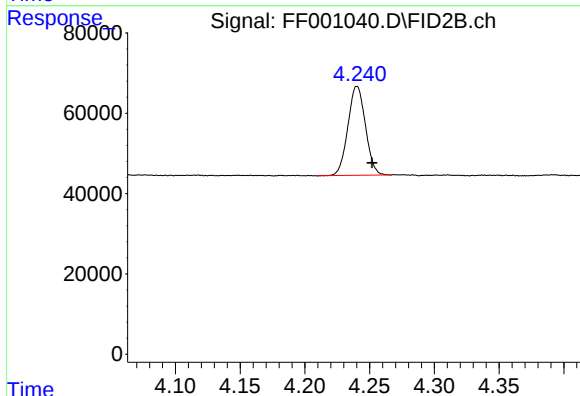


#2 N-DECANE

R.T.: 4.240 min
Delta R.T.: -0.011 min
Response: 209247
Conc: 1.49 ug/ml

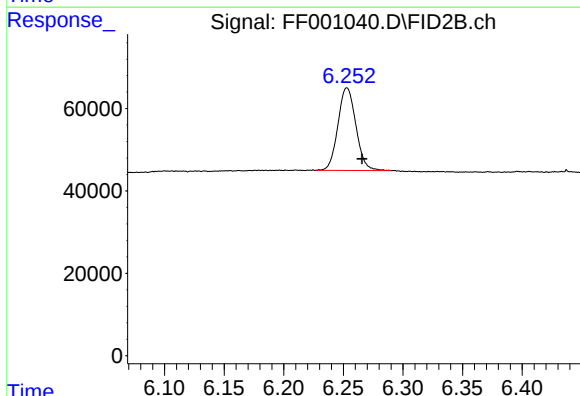


#3 N-DODECANE

R.T.: 6.253 min
Delta R.T.: -0.013 min
Response: 210659
Conc: 1.50 ug/ml

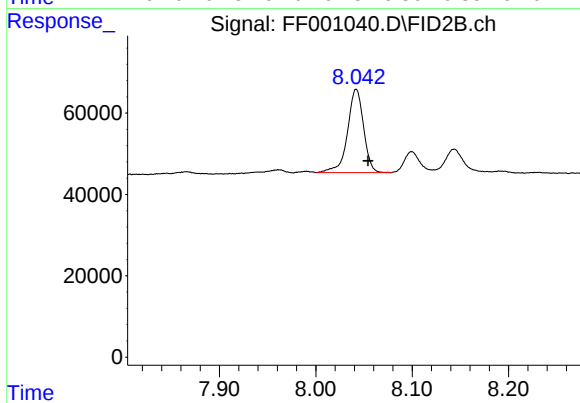

#4 N-TETRADECANE


R.T.: 8.042 min
Delta R.T.: -0.012 min
Response: 235962
Conc: 1.69 ug/ml

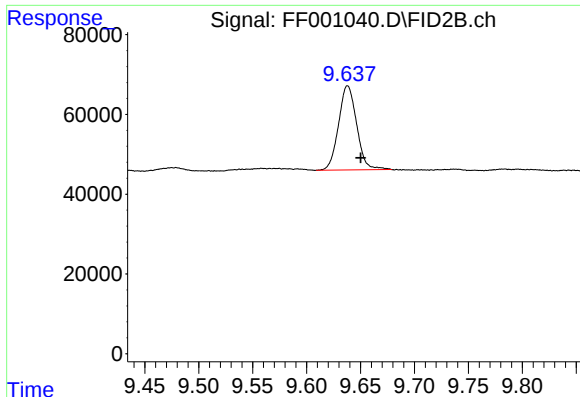

#5 N-HEXADECANE


R.T.: 9.638 min
Delta R.T.: -0.012 min
Response: 246944
Conc: 1.79 ug/ml

Instrument :
FID_F
ClientSampleId :

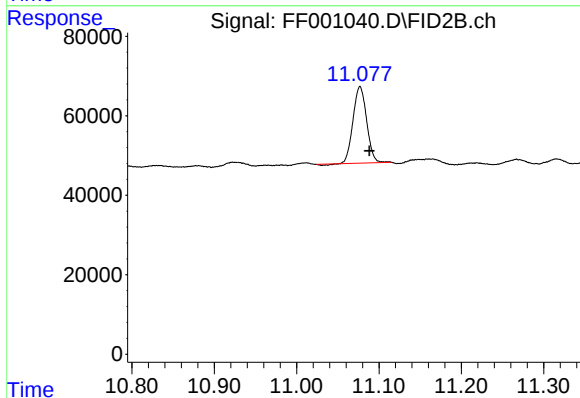


#6 N-OCTADECANE

R.T.: 11.077 min
Delta R.T.: -0.011 min
Response: 222212
Conc: 1.63 ug/ml

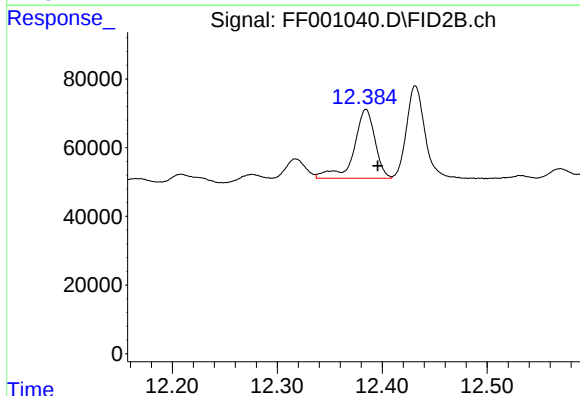


#7 N-EICOSANE

R.T.: 12.385 min
Delta R.T.: -0.011 min
Response: 280507
Conc: 2.09 ug/ml

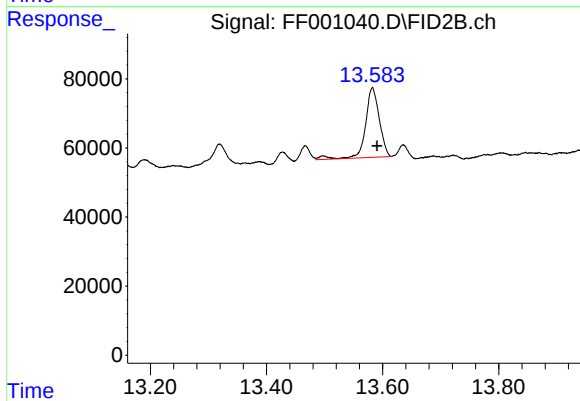

#8 N-DOCOSANE


R.T.: 13.582 min
Delta R.T.: -0.008 min
Response: 333742
Conc: 2.52 ug/ml

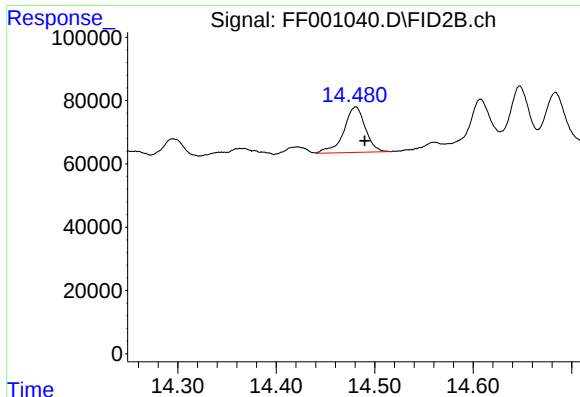

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.481 min
Delta R.T.: -0.009 min
Response: 218985
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :

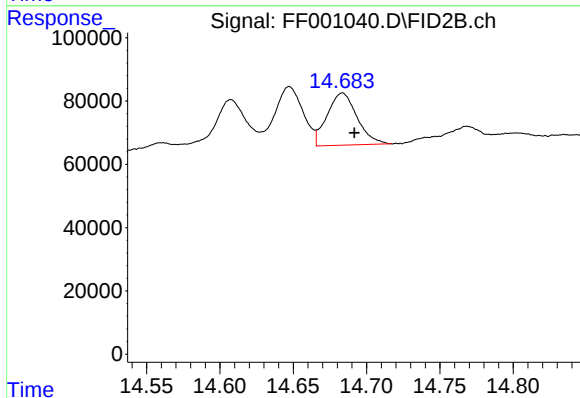


#10 N-TETRACOSANE

R.T.: 14.684 min
Delta R.T.: -0.008 min
Response: 234517
Conc: 1.81 ug/ml

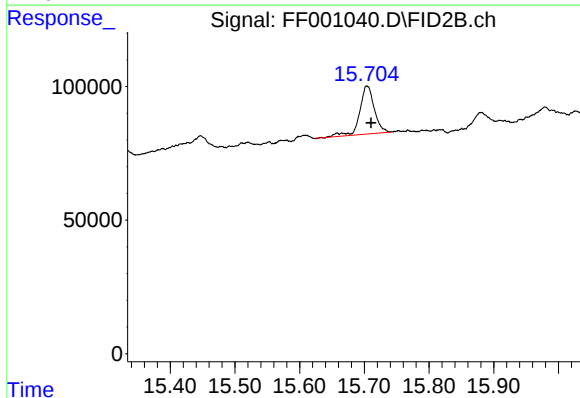


#11 N-HEXACOSANE

R.T.: 15.704 min
Delta R.T.: -0.007 min
Response: 278731
Conc: 2.17 ug/ml

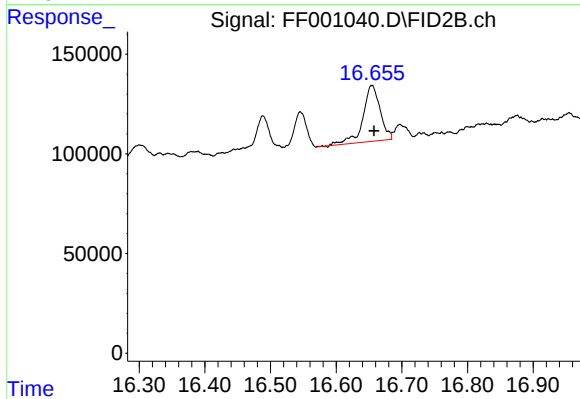

#12 N-OCTACOSANE


R.T.: 16.654 min
Delta R.T.: -0.003 min
Response: 512866
Conc: 4.03 ug/ml

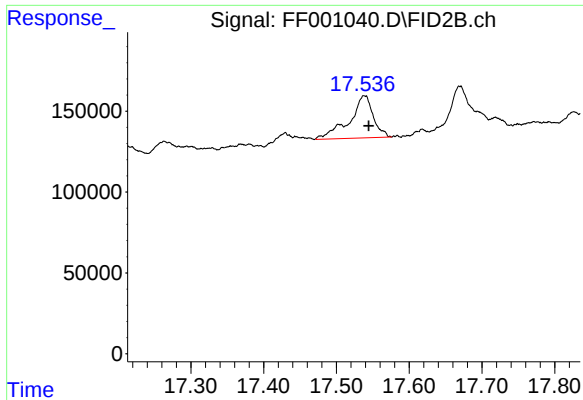

#13 N-TRIACONTANE


R.T.: 17.538 min
Delta R.T.: -0.006 min
Response: 597320
Conc: 4.73 ug/ml

Instrument :
FID_F
ClientSampleId :

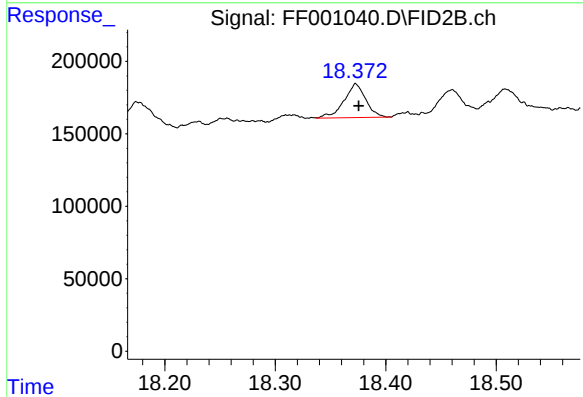


#14 N-DOTRIACONTANE

R.T.: 18.373 min
Delta R.T.: -0.002 min
Response: 316902
Conc: 2.58 ug/ml

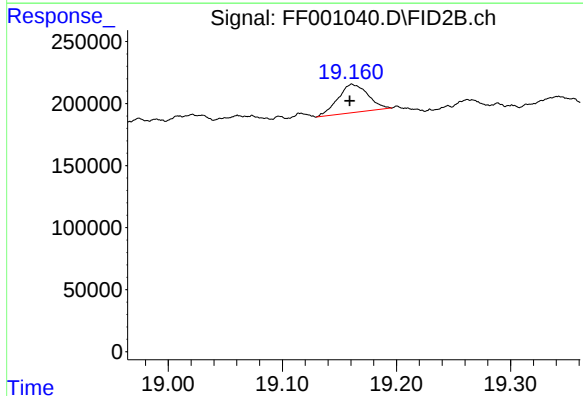


#15 N-TETRATRIACONTANE

R.T.: 19.161 min
Delta R.T.: 0.002 min
Response: 415562
Conc: 3.46 ug/ml

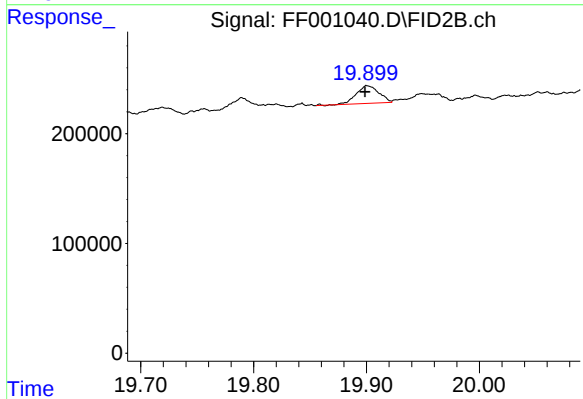

#16 N-HEXATRIACONTANE

R.T.: 19.901 min
Delta R.T.: 0.002 min
Response: 226669
Conc: 1.99 ug/ml

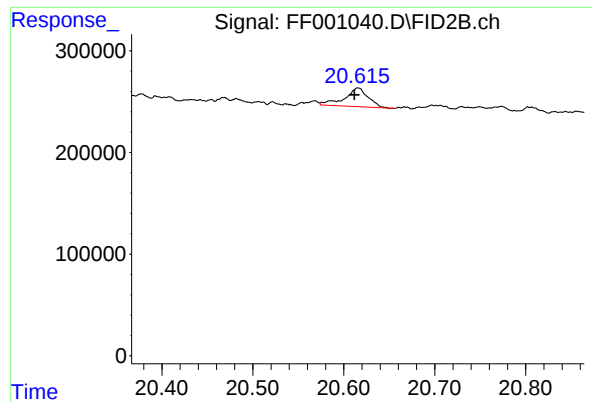

#17 N-OCTATRIACONTANE

R.T.: 20.616 min
Delta R.T.: 0.004 min
Response: 328344
Conc: 3.19 ug/ml

Instrument :
FID_F
ClientSampleId :