

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
 Data File : FF001026.D
 Signal(s) : FID2B.ch
 Acq On : 20 Jun 2018 10:11
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jun 21 07:49:15 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.483	5615390	48.692 ug/ml
Target Compounds			
2) N-DECANE	4.243	7840463	55.957 ug/ml
3) N-DODECANE	6.257	7440032	53.085 ug/ml
4) N-TETRADECANE	8.046	7134523	51.243 ug/ml
5) N-HEXADECANE	9.642	6887531	49.954 ug/ml
6) N-OCTADECANE	11.081	6706120	49.110 ug/ml
7) N-EICOSANE	12.388	6512097	48.606 ug/ml
8) N-DOCOSANE	13.584	6397293	48.381 ug/ml
10) N-TETRACOSANE	14.687	6365130	49.072 ug/ml
11) N-HEXACOSANE	15.707	6369917	49.593 ug/ml
12) N-OCTACOSANE	16.654	6459774	50.801 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001026.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 10:11
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Jun 21 07:49:15 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

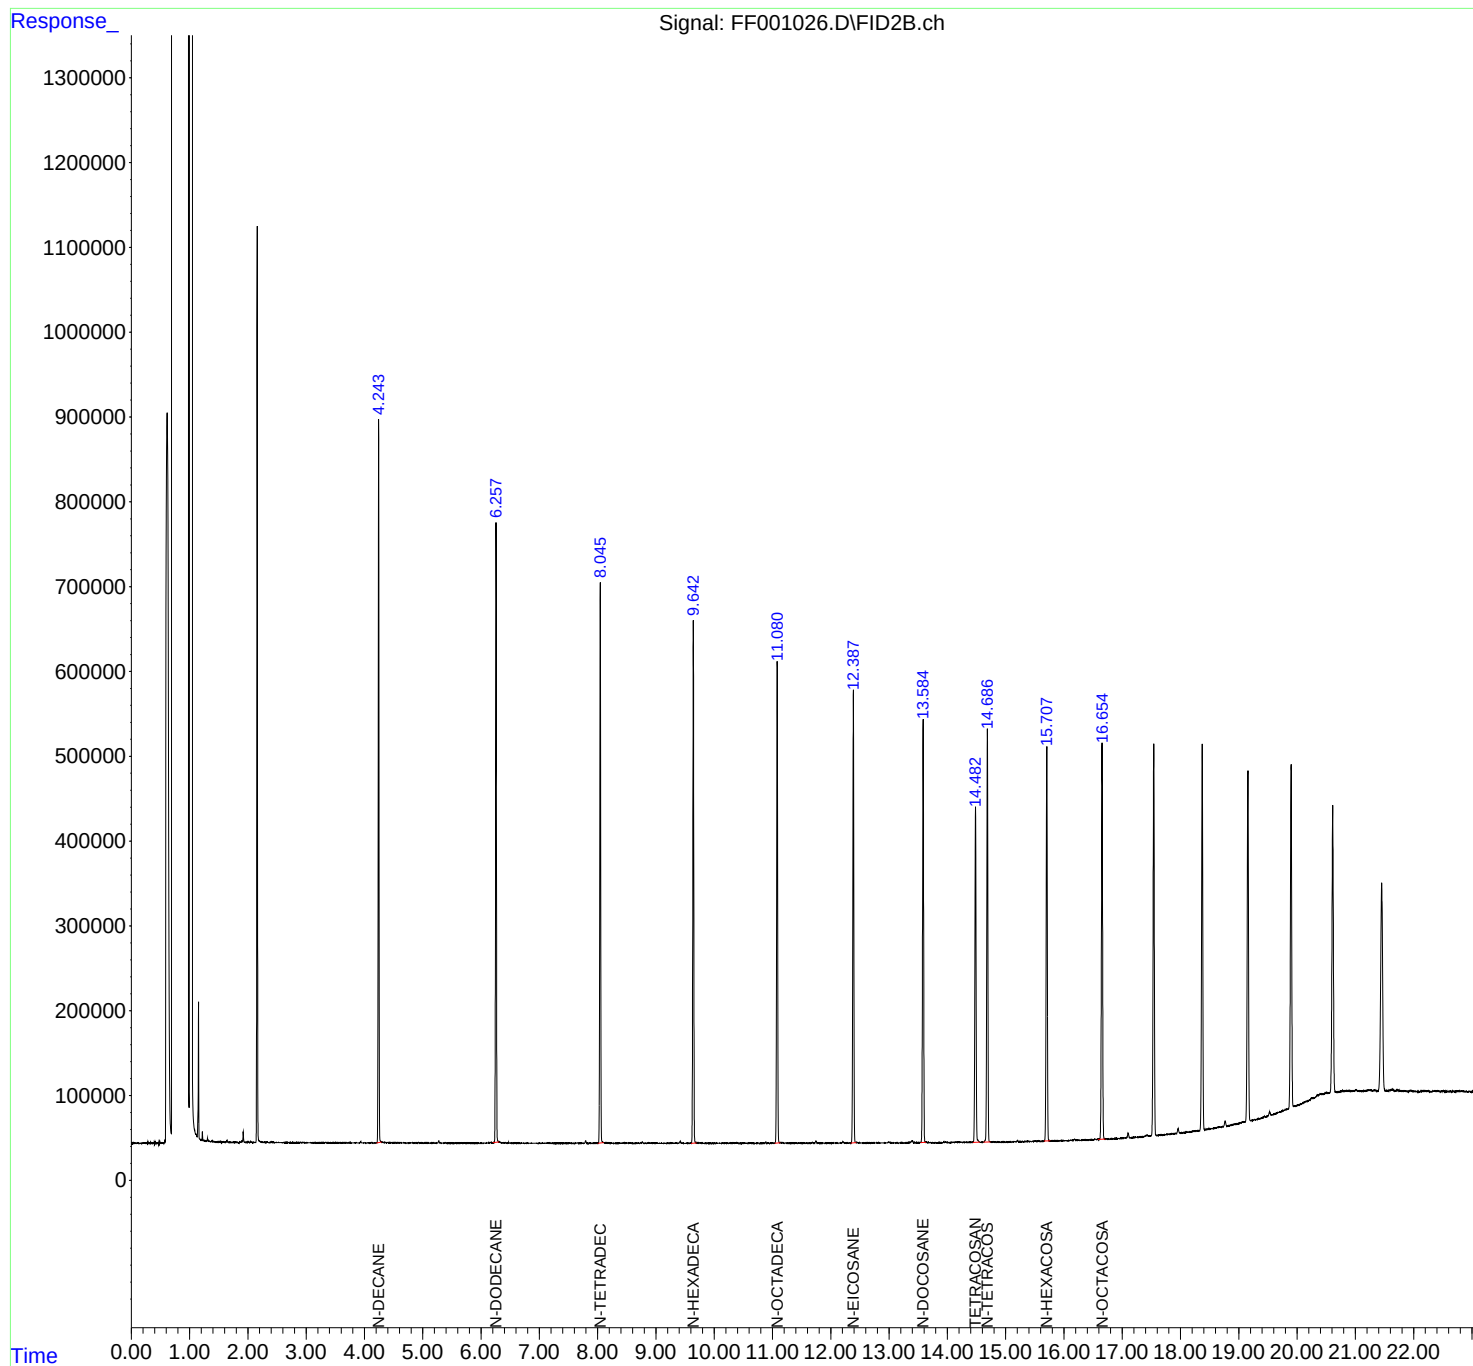


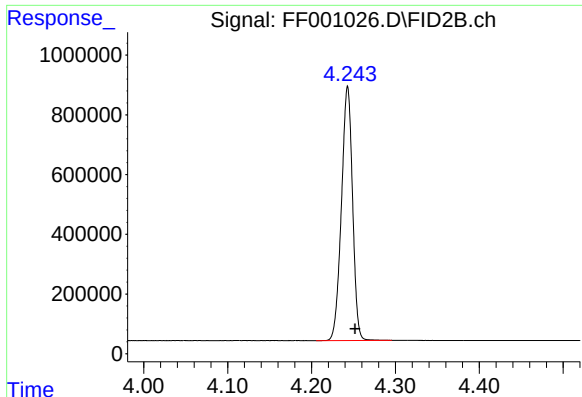

#2 N-DECANE


R.T.: 4.243 min
Delta R.T.: -0.009 min
Response: 7840463
Conc: 55.96 ug/ml

Instrument :
FID_F
ClientSampleId :

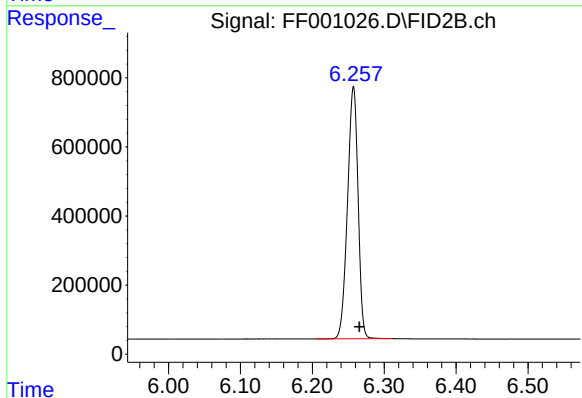


#3 N-DODECANE

R.T.: 6.257 min
Delta R.T.: -0.008 min
Response: 7440032
Conc: 53.09 ug/ml

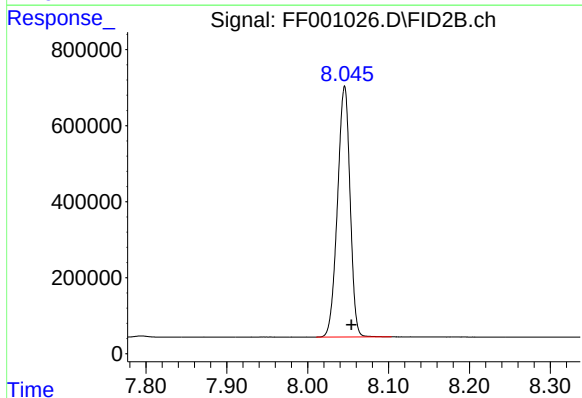


#4 N-TETRADECANE

R.T.: 8.046 min
Delta R.T.: -0.008 min
Response: 7134523
Conc: 51.24 ug/ml

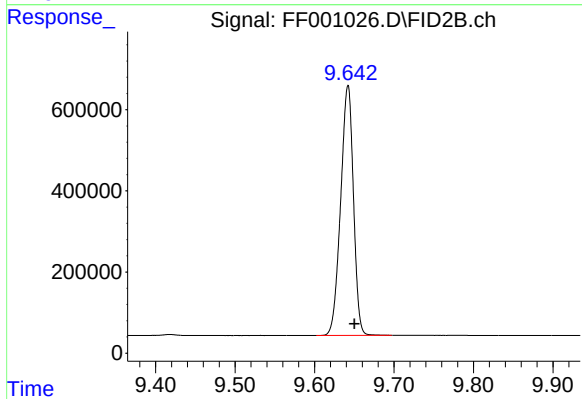

#5 N-HEXADECANE


R.T.: 9.642 min
Delta R.T.: -0.008 min
Response: 6887531
Conc: 49.95 ug/ml

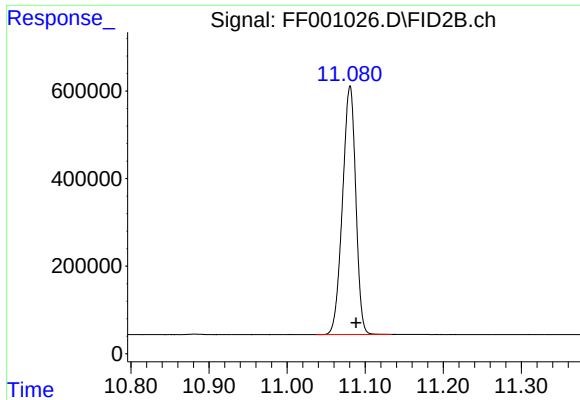

#6 N-OCTADECANE


R.T.: 11.081 min
Delta R.T.: -0.008 min
Response: 6706120
Conc: 49.11 ug/ml

Instrument :
FID_F
ClientSampleId :

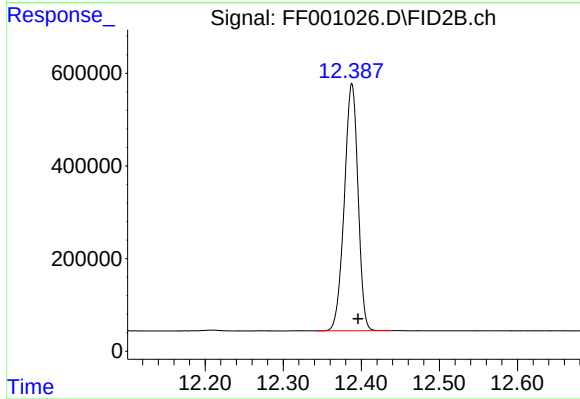


#7 N-EICOSANE

R.T.: 12.388 min
Delta R.T.: -0.008 min
Response: 6512097
Conc: 48.61 ug/ml

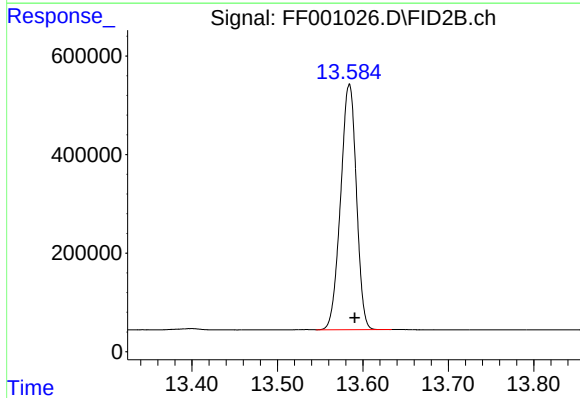


#8 N-DOCOSANE

R.T.: 13.584 min
Delta R.T.: -0.006 min
Response: 6397293
Conc: 48.38 ug/ml

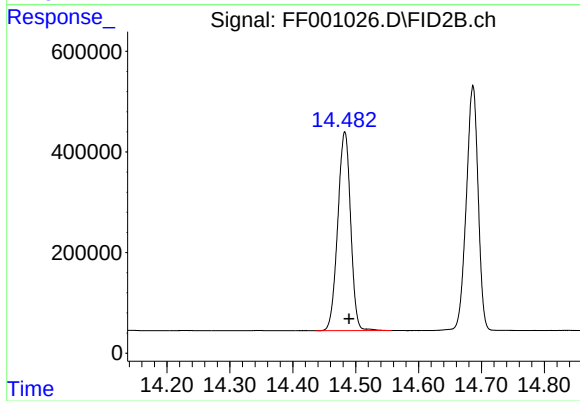

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.483 min
Delta R.T.: -0.007 min
Response: 5615390
Conc: 48.69 ug/ml

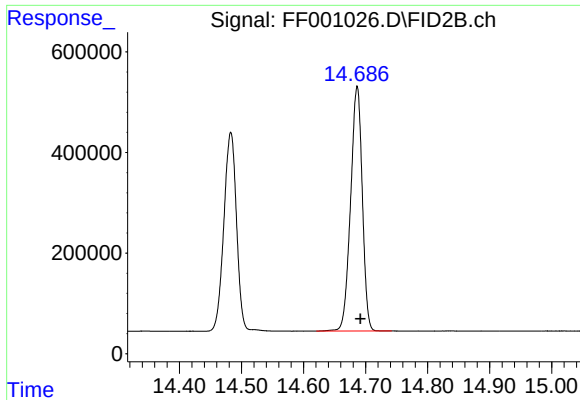

#10 N-TETRACOSANE


R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 6365130
Conc: 49.07 ug/ml

Instrument :
FID_F
ClientSampleId :

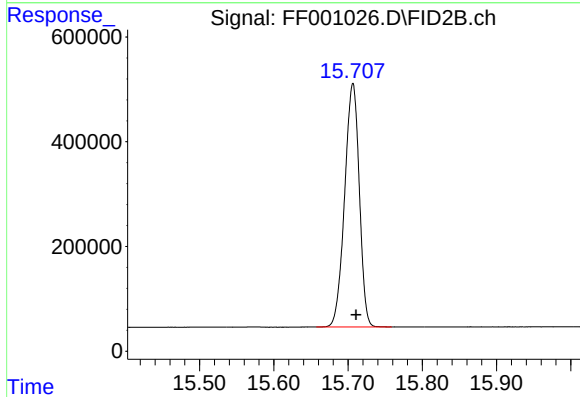

#11 N-HEXACOSANE

R.T.: 15.707 min
Delta R.T.: -0.004 min
Response: 6369917
Conc: 49.59 ug/ml

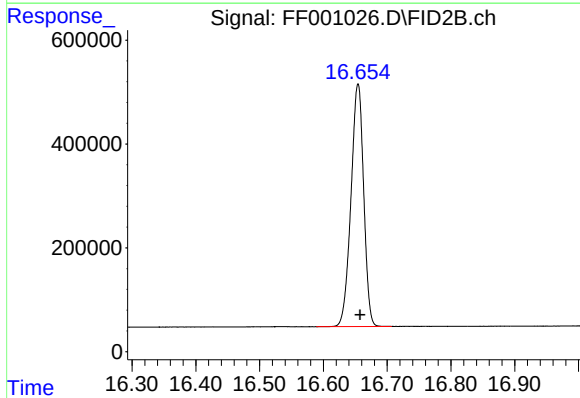

#12 N-OCTACOSANE

R.T.: 16.654 min
Delta R.T.: -0.003 min
Response: 6459774
Conc: 50.80 ug/ml