

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001032.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 13:10
Operator : UA\AJ
Sample : J3249-03 20X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

UGO
6/21/2018 3:19:04 PM

Integration File: Sample.e
Quant Time: Jun 21 07:51:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.477	256668	2.226 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062018\
Data File : FF001032.D
Signal(s) : FID2B.ch
Acq On : 20 Jun 2018 13:10
Operator : UA\AJ
Sample : J3249-03 20X
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :


Manual Integrations
APPROVED

UGO
6/21/2018 3:19:04 PM

Integration File: Sample.e
Quant Time: Jun 21 07:51:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

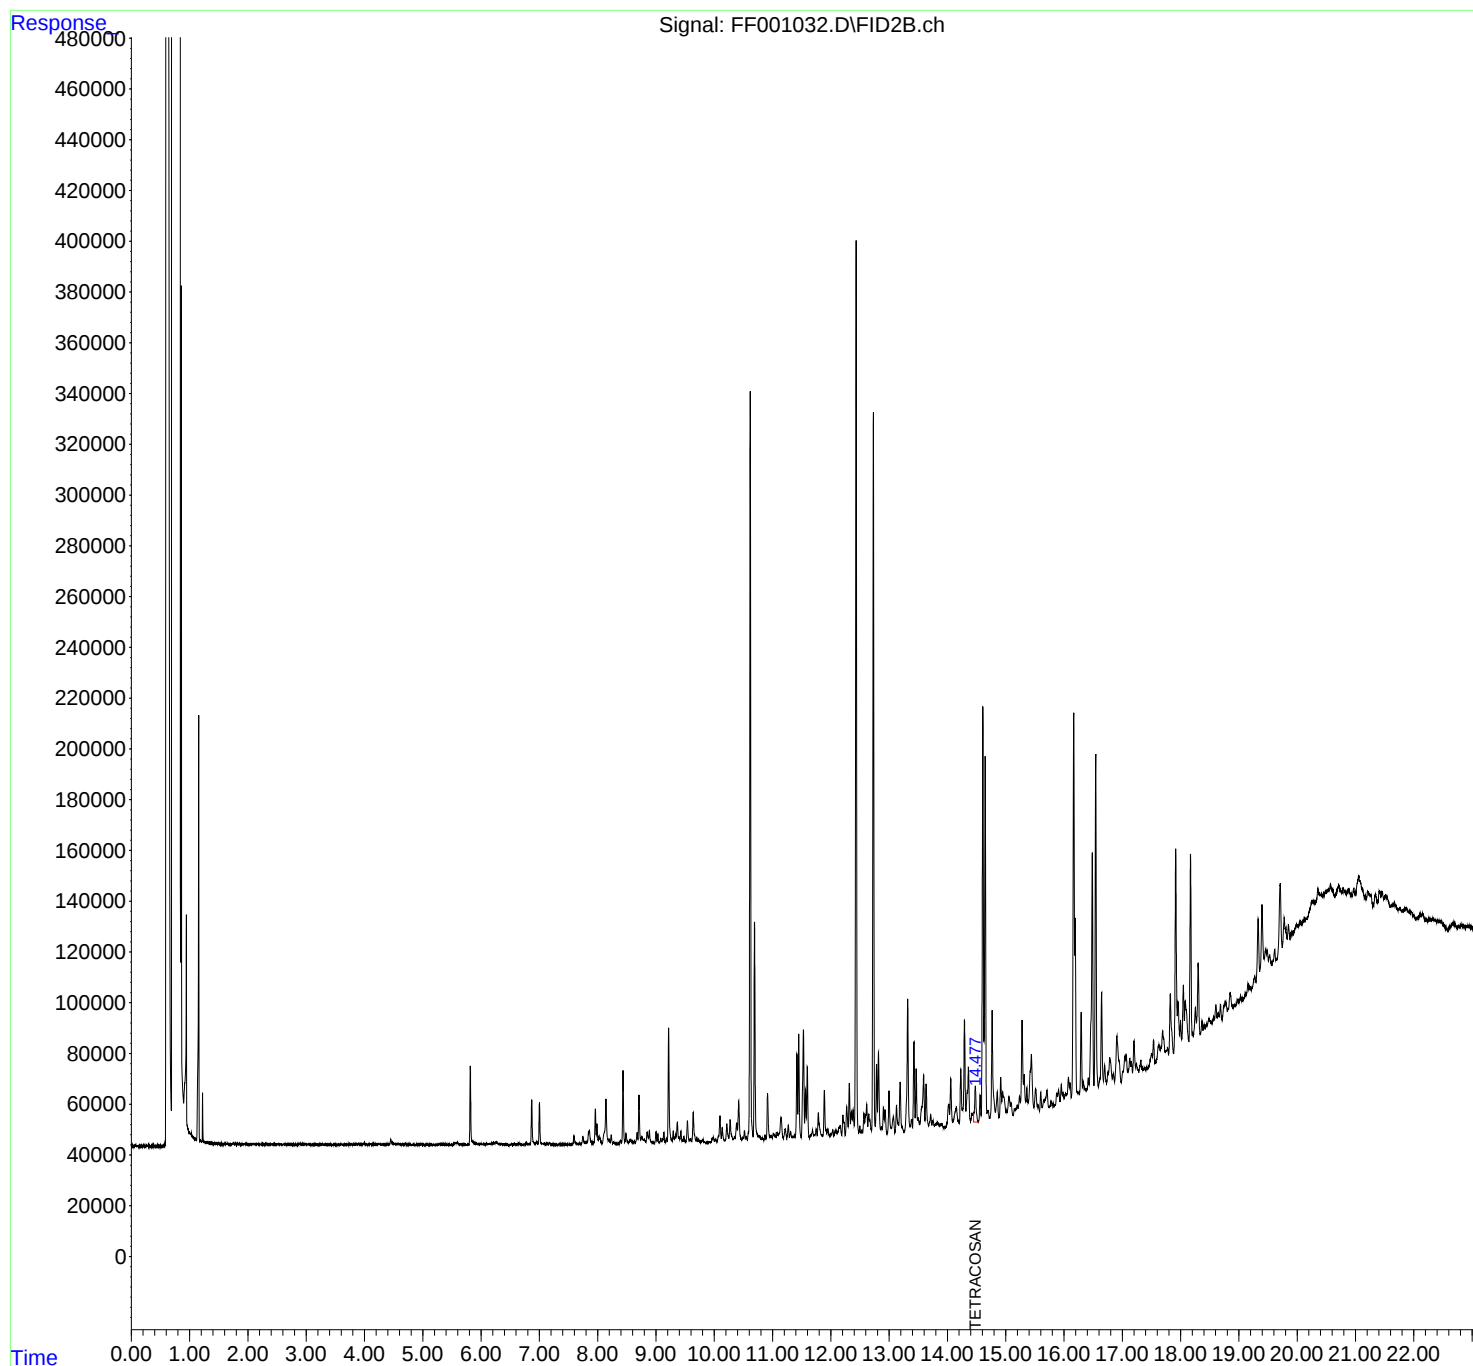

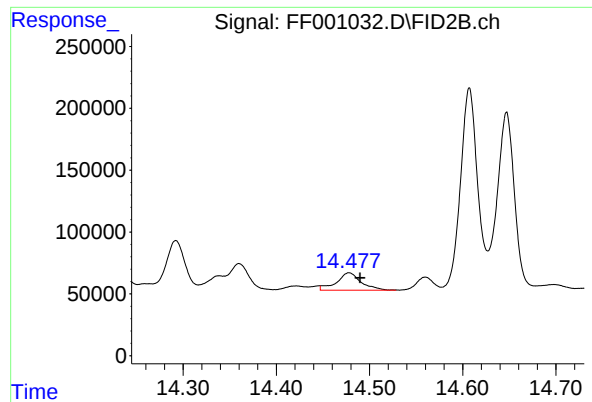

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.477 min
Delta R.T.: -0.012 min
Response: 256668
Conc: 2.23 ug/ml m

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

UGO
6/21/2018 3:19:04 PM