

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062220\
Data File : FF007094.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2020 17:51
Operator : DD\AJ
Sample : L3080-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JFK-GW-01-15-D

Integration File: Sample.e
Quant Time: Jun 23 01:17:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.744	2186651	18.575 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062220\
Data File : FF007094.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2020 17:51
Operator : DD\AJ
Sample : L3080-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JFK-GW-01-15-D

Integration File: Sample.e
Quant Time: Jun 23 01:17:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

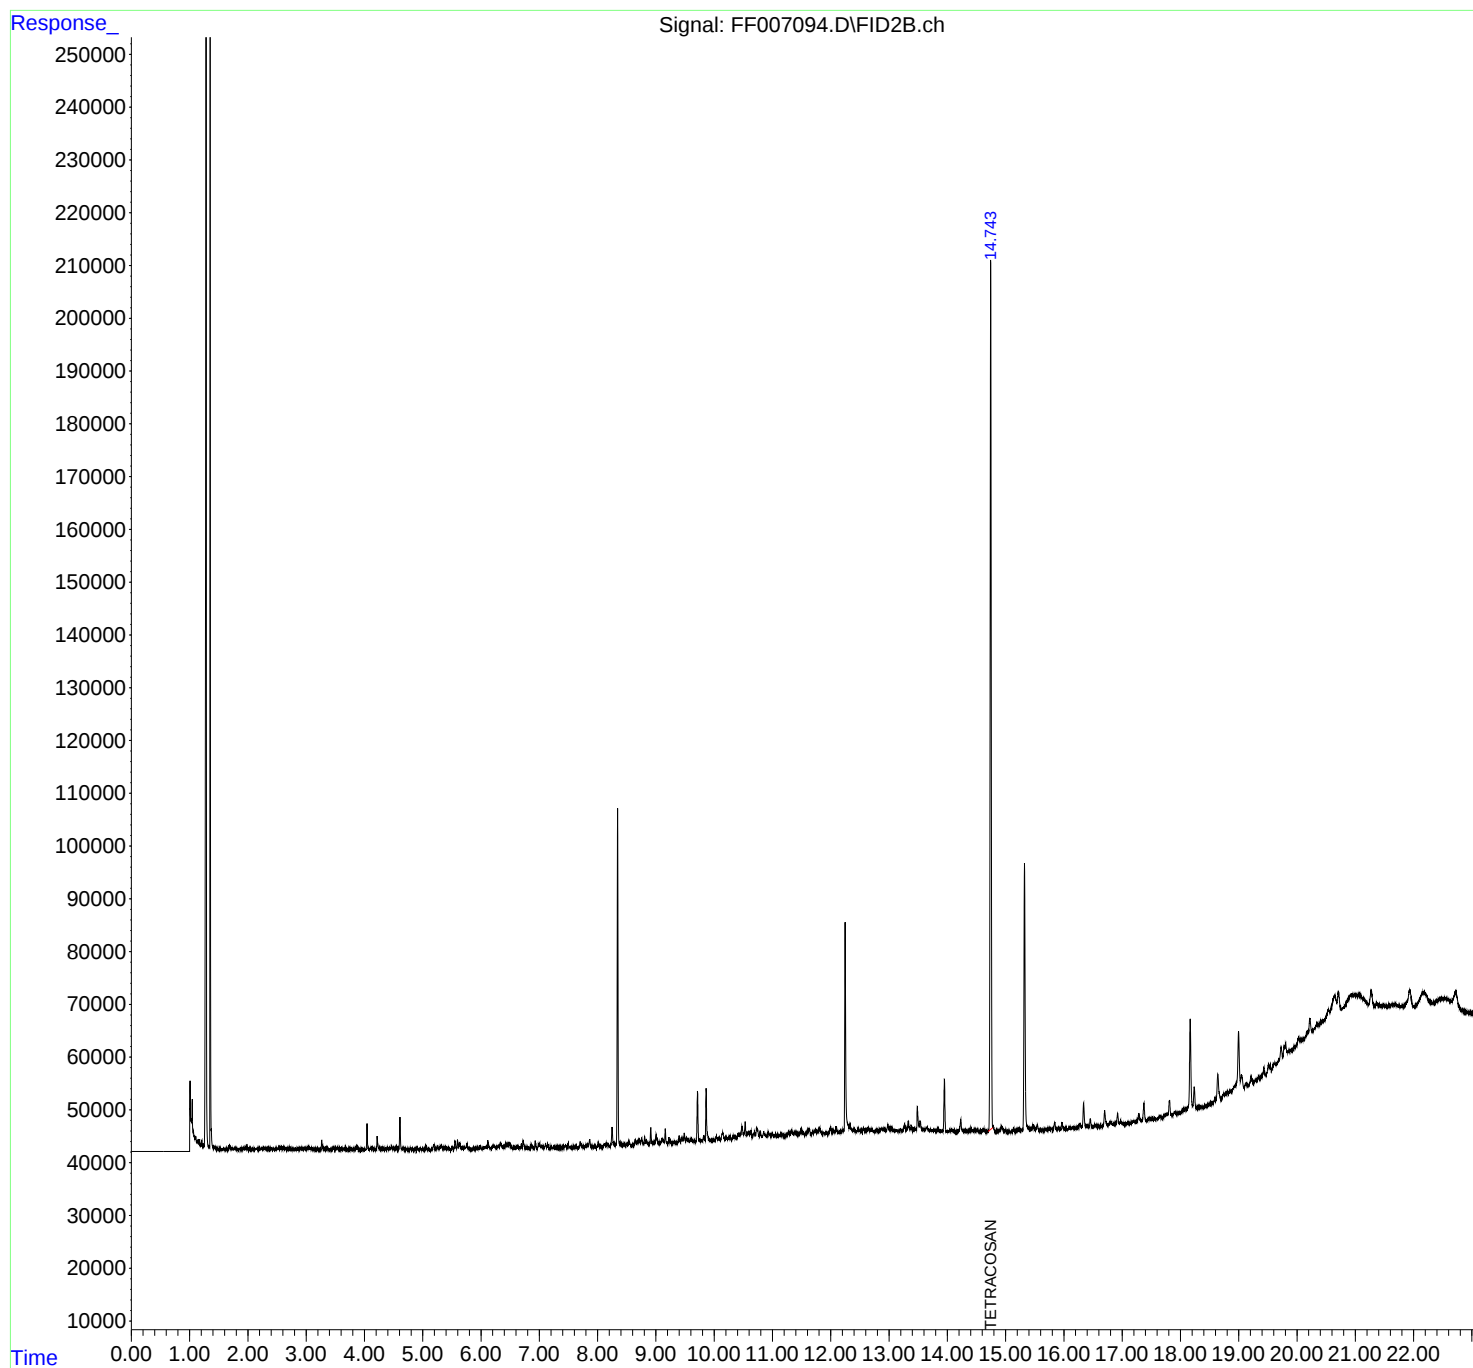

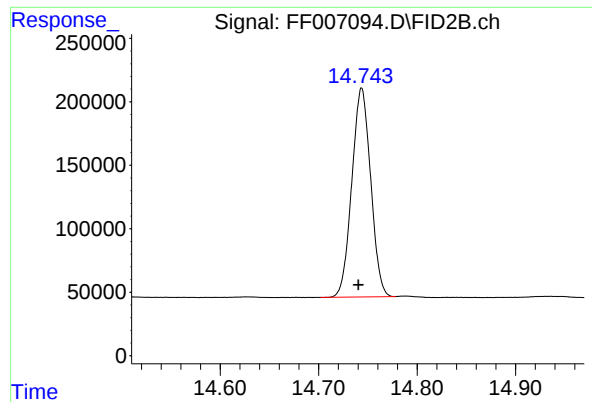

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.744 min
Delta R.T.: 0.003 min
Response: 2186651
Conc: 18.58 ug/ml

Instrument :
FID_F
ClientSampleId :
JFK-GW-01-15-D