

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010811.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 14:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 01:08:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.730	253577	2.090 ug/ml
16)	N-HEXATRIACONTANE	20.277f	533754	6.207 ug/ml
18)	N-TETRACONTANE	21.805	950197	12.161 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010811.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 14:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 01:08:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

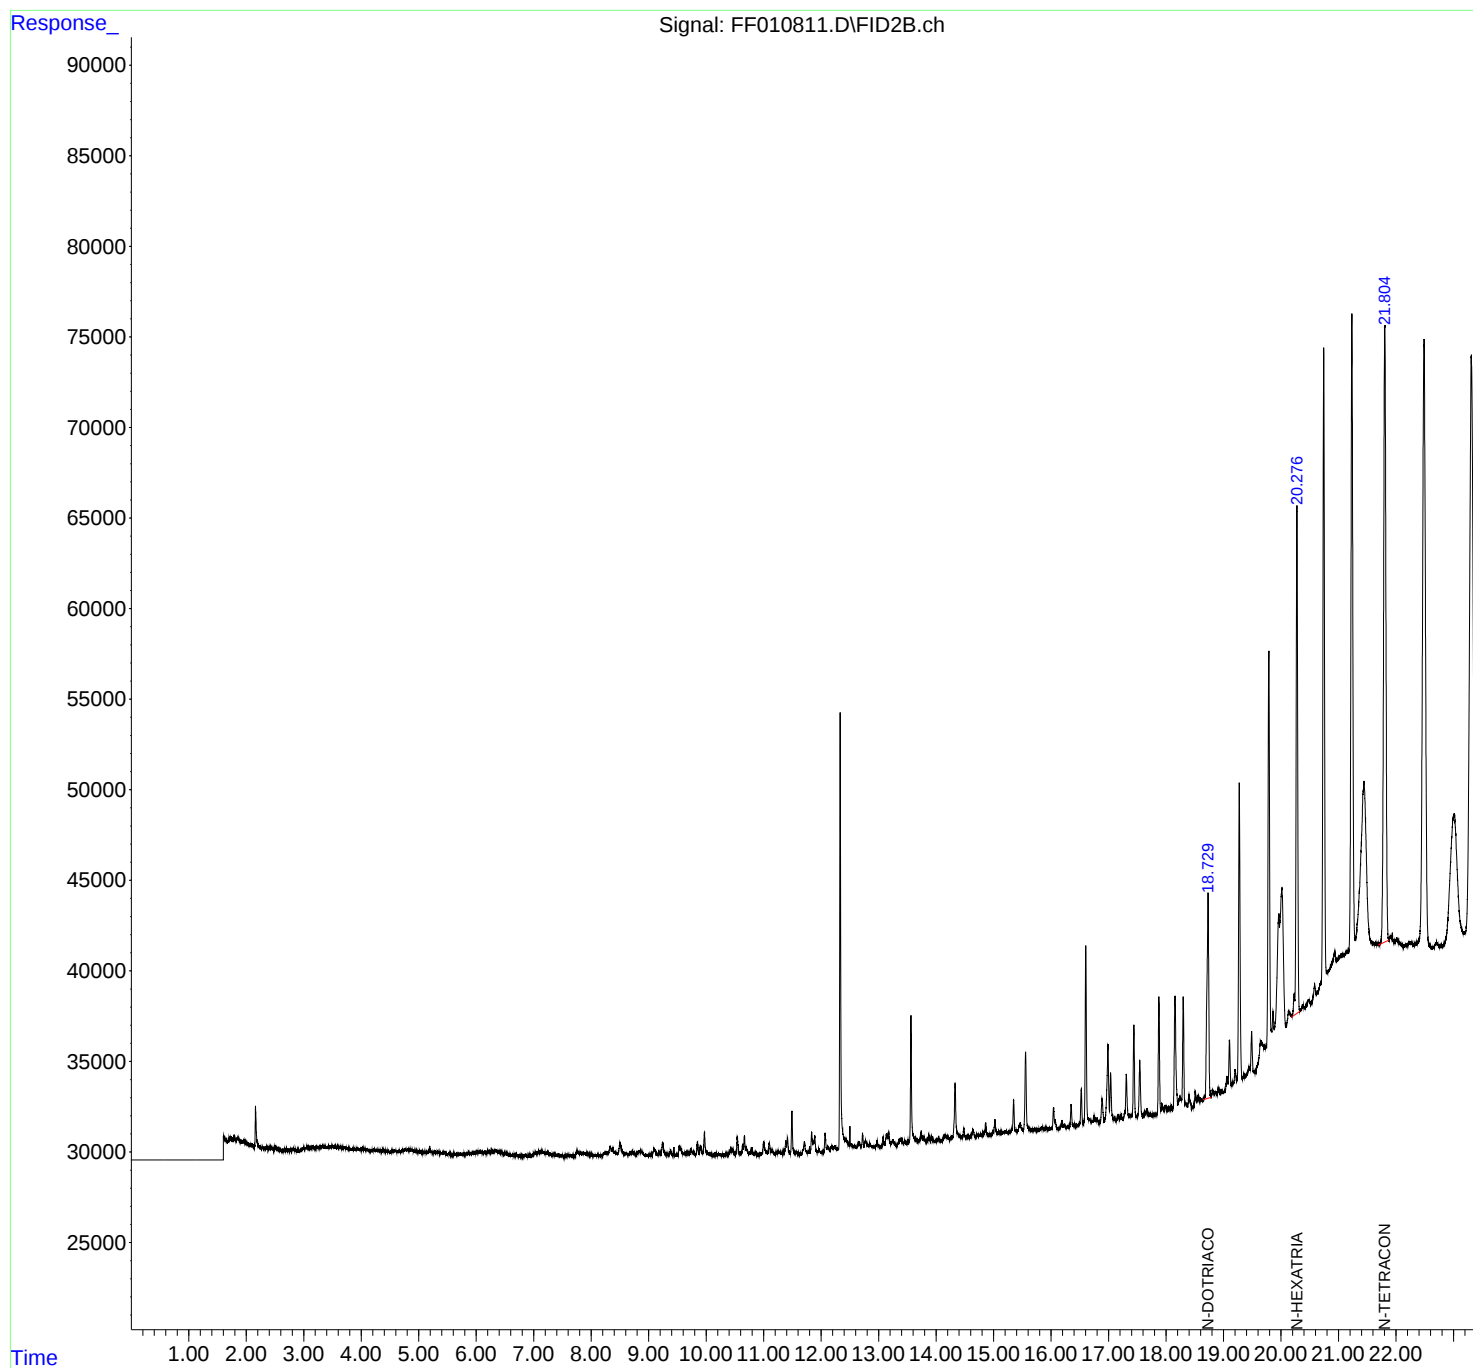


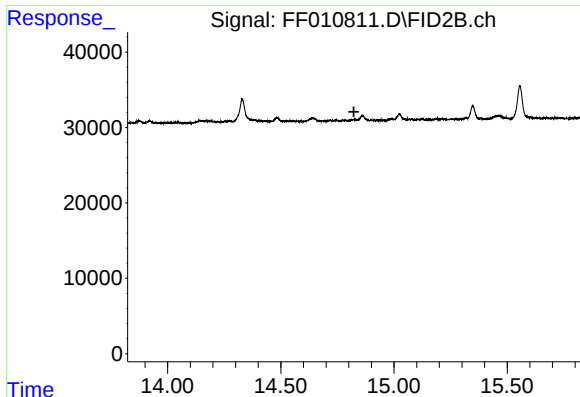

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.823 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

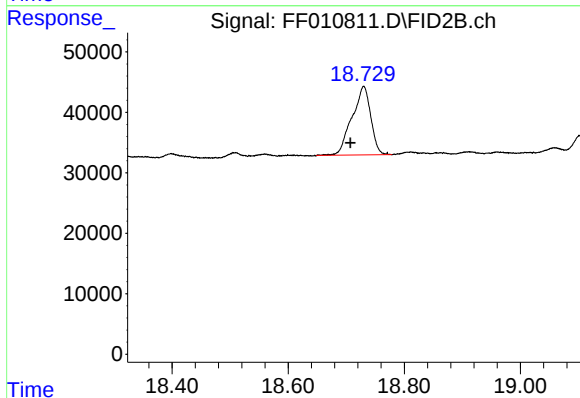


#14 N-DOTRIACONTANE

R.T.: 18.730 min
Delta R.T.: 0.023 min
Response: 253577
Conc: 2.09 ug/ml

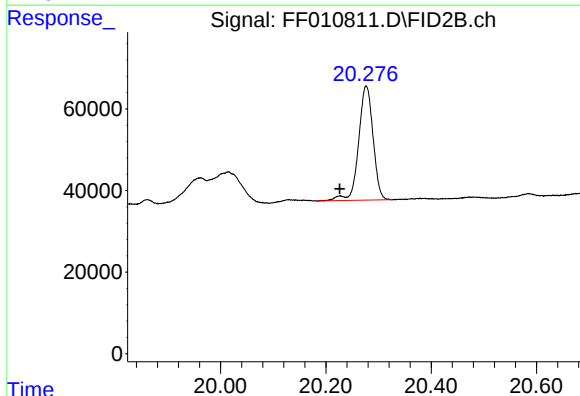

#16 N-HEXATRIACONTANE

R.T.: 20.277 min
Delta R.T.: 0.051 min
Response: 533754
Conc: 6.21 ug/ml

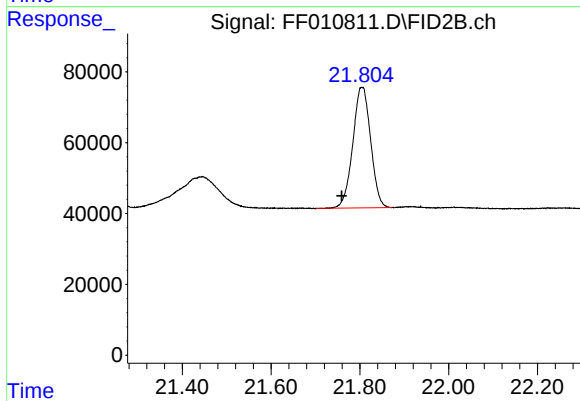

#18 N-TETRACONTANE

R.T.: 21.805 min
Delta R.T.: 0.045 min
Response: 950197
Conc: 12.16 ug/ml