

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062222\  
Data File : FF010812.D  
Signal(s) : FID2B.ch  
Acq On : 22 Jun 2022 15:03  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 23 01:09:20 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.819 | 2210296  | 19.554 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.707 | 133216   | 1.098 ug/ml  |
| 18) N-TETRACONTANE            | 21.801 | 190915   | 2.443 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062222\  
Data File : FF010812.D  
Signal(s) : FID2B.ch  
Acq On : 22 Jun 2022 15:03  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 23 01:09:20 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

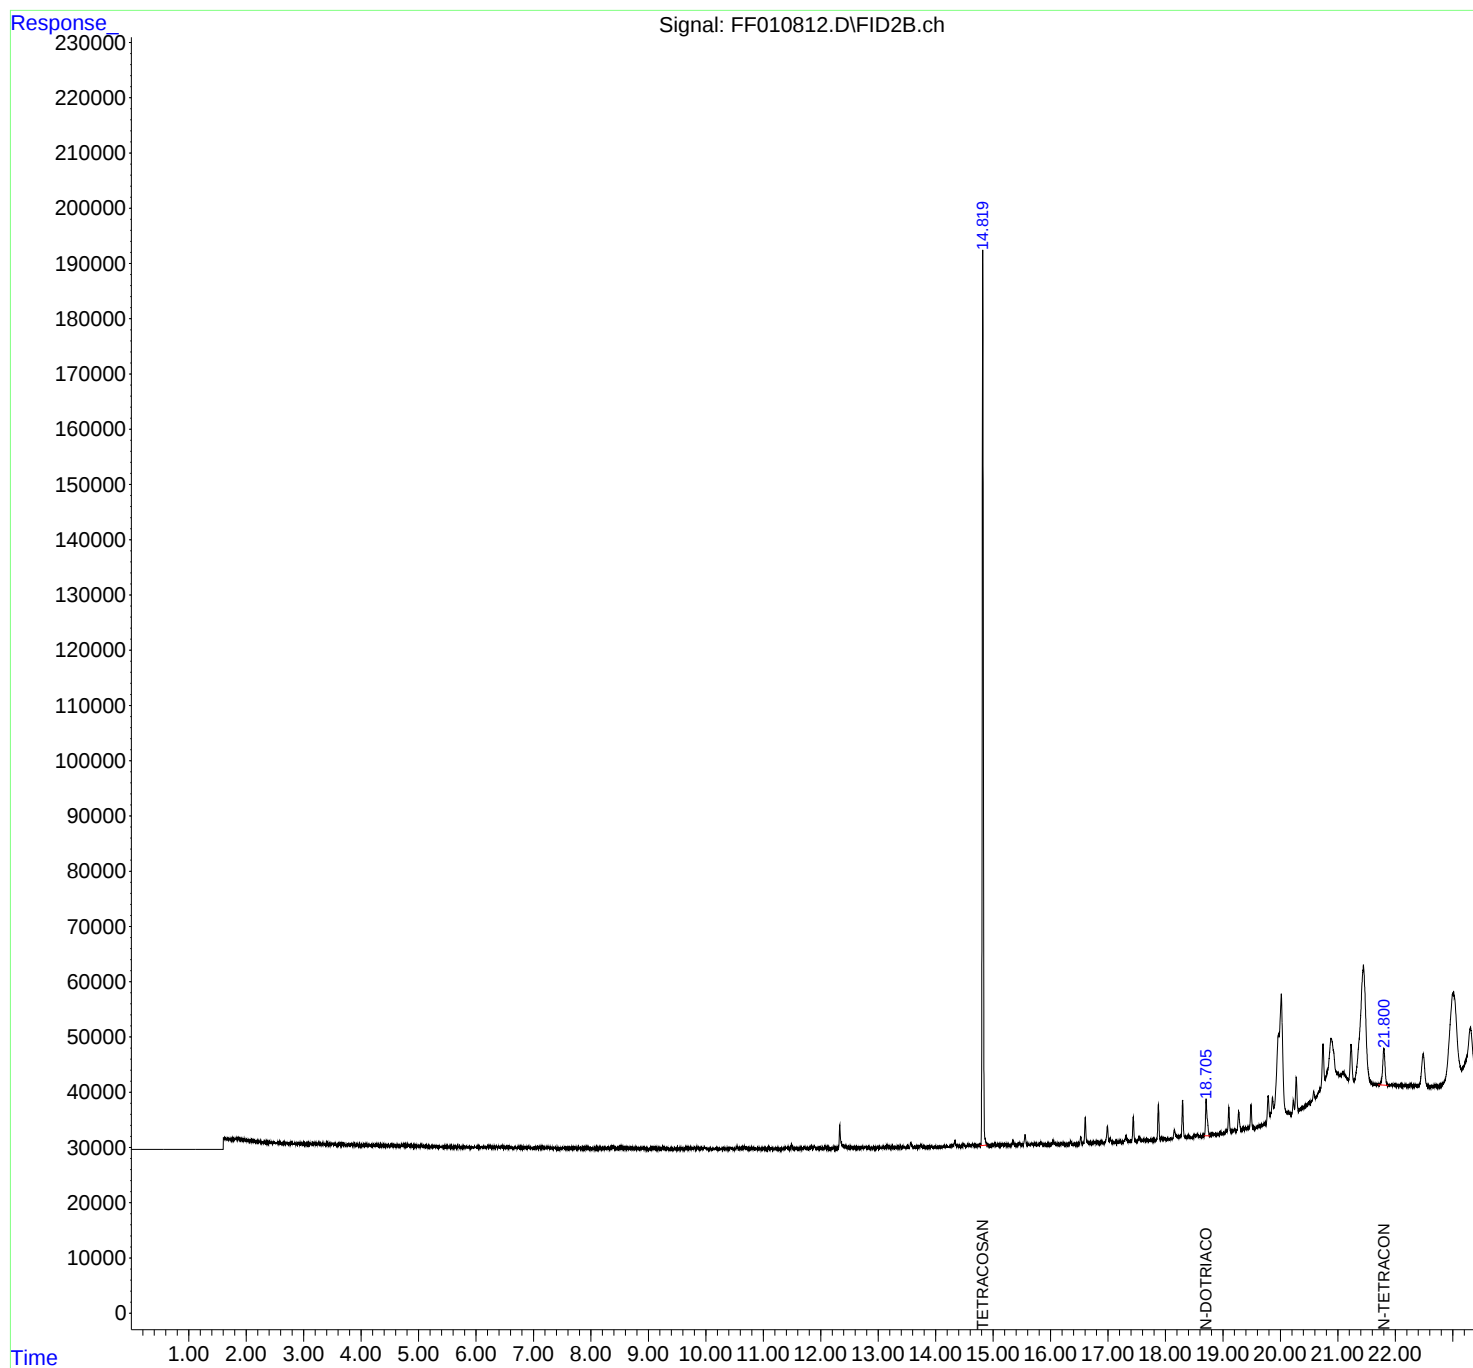


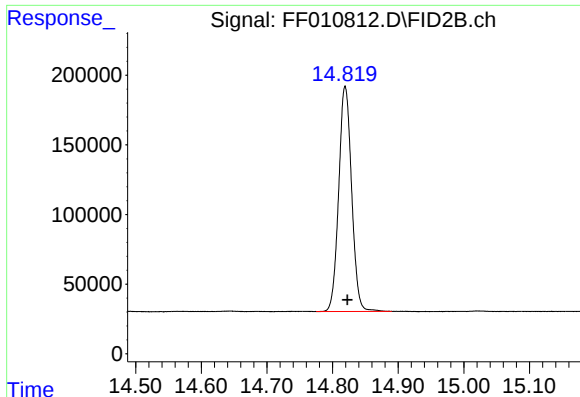

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.819 min  
Delta R.T.: -0.004 min  
Response: 2210296  
Conc: 19.55 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

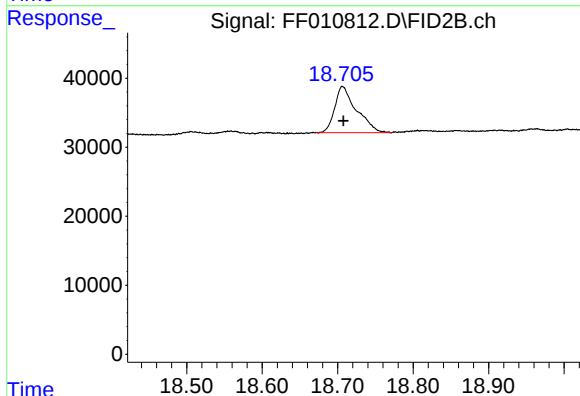

#14 N-DOTRIACONTANE

R.T.: 18.707 min  
Delta R.T.: 0.000 min  
Response: 133216  
Conc: 1.10 ug/ml

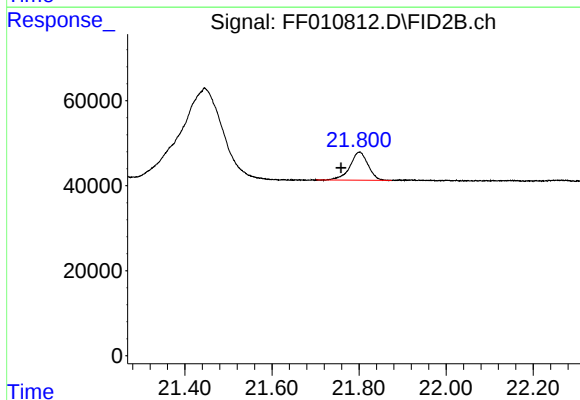

#18 N-TETRACONTANE

R.T.: 21.801 min  
Delta R.T.: 0.042 min  
Response: 190915  
Conc: 2.44 ug/ml