

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
 Data File : FF010825.D
 Signal(s) : FID2B.ch
 Acq On : 22 Jun 2022 21:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 23 01:17:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.827	2137390	18.909 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.883	234982	1.917 ug/ml
14) N-DOTRIACONTANE	18.713	177506	1.463 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010825.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 21:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 01:17:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

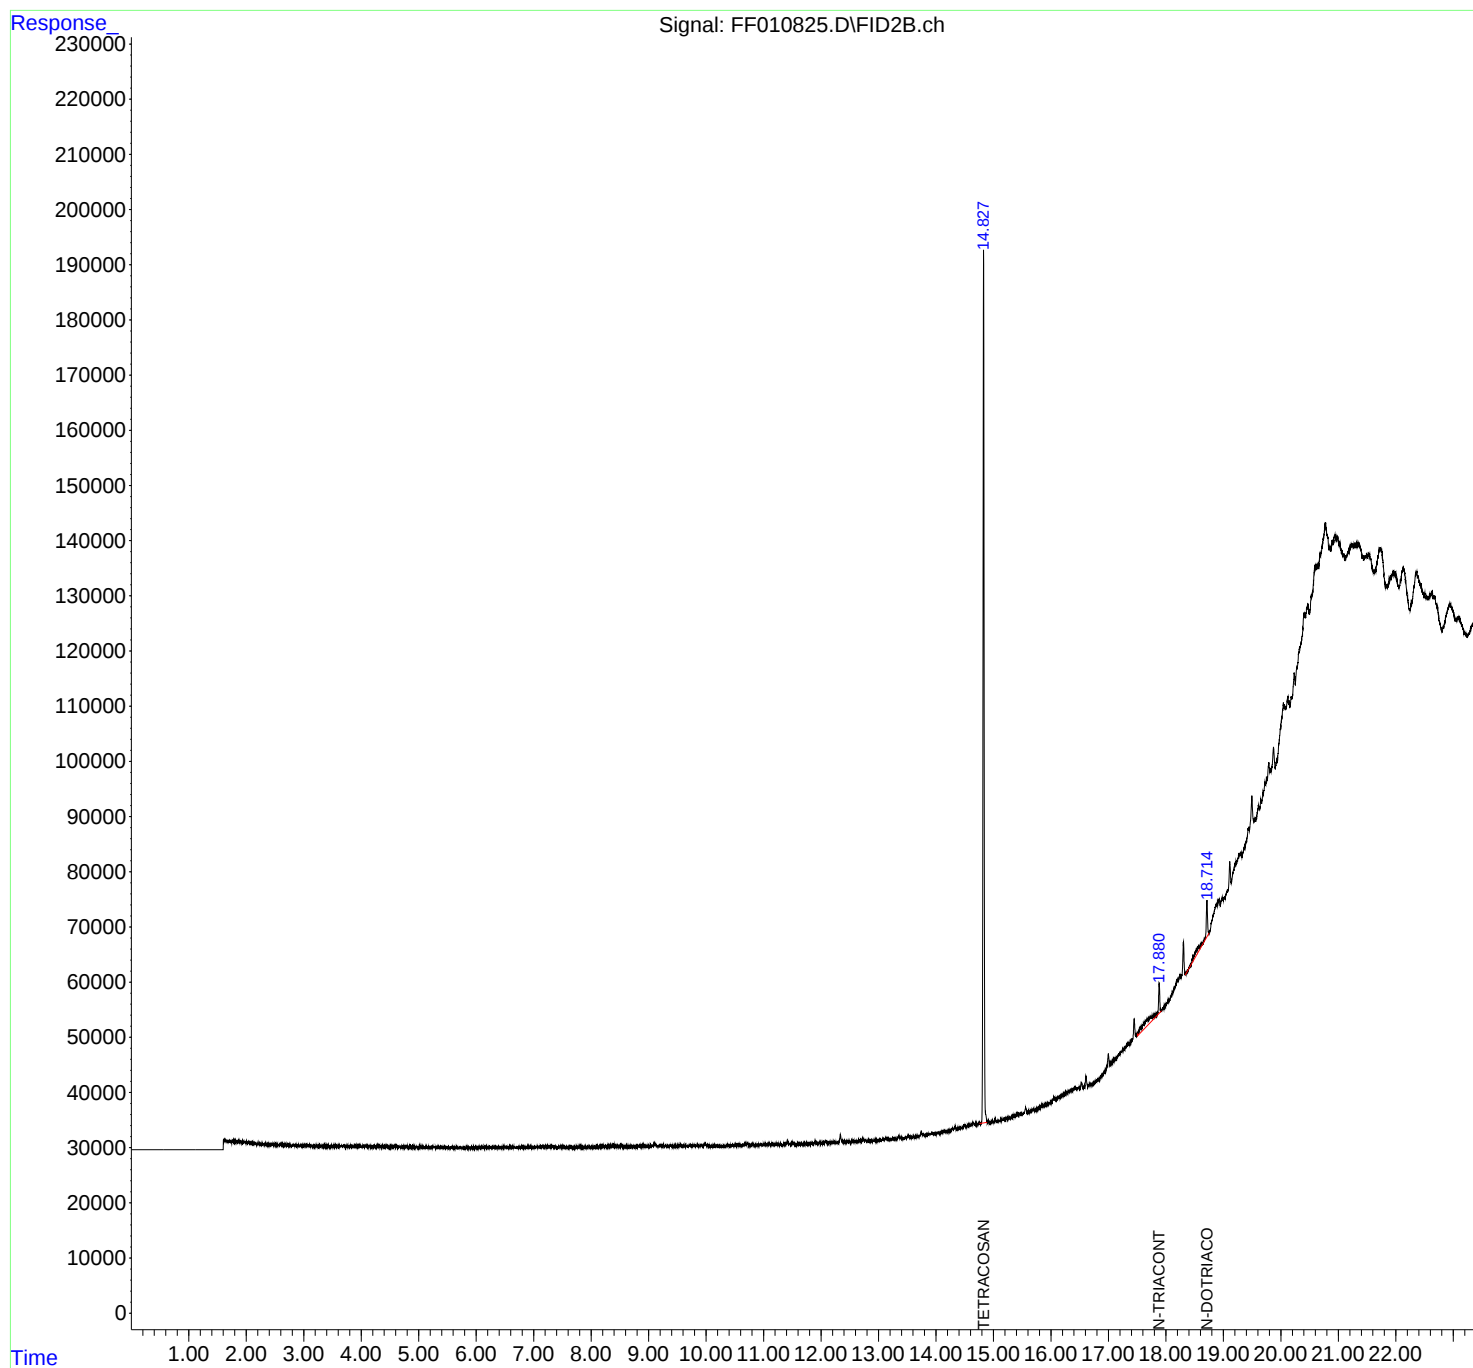


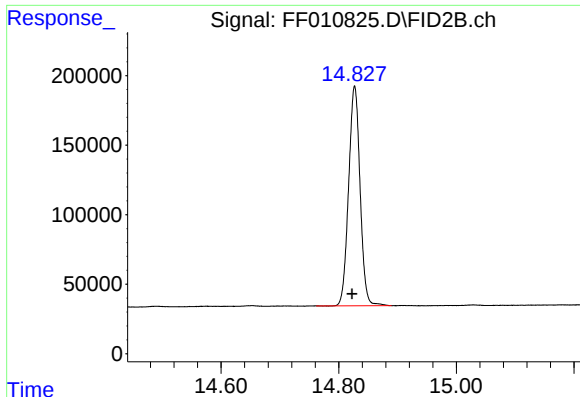

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.827 min
Delta R.T.: 0.004 min
Response: 2137390
Conc: 18.91 ug/ml

Instrument :
FID_F
ClientSampleId :

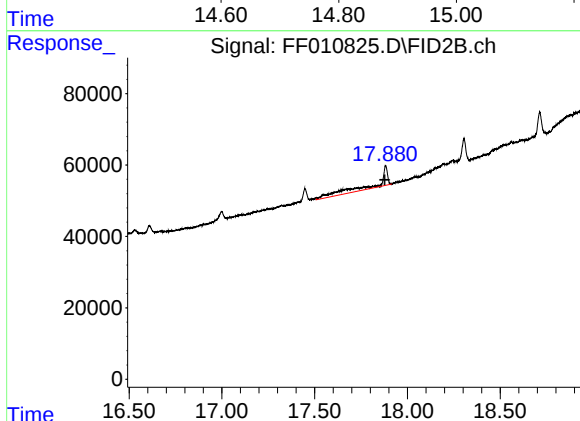

#13 N-TRIACONTANE

R.T.: 17.883 min
Delta R.T.: 0.006 min
Response: 234982
Conc: 1.92 ug/ml

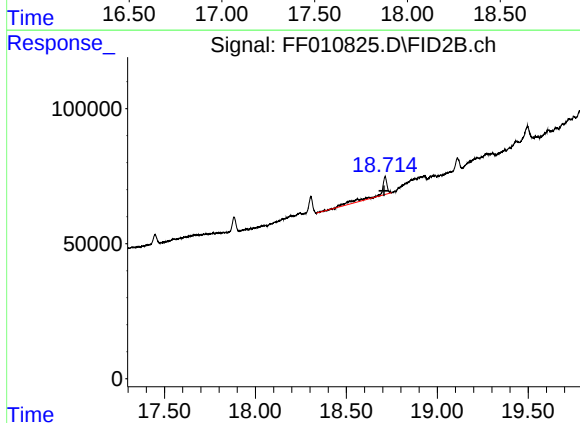

#14 N-DOTRIACONTANE

R.T.: 18.713 min
Delta R.T.: 0.006 min
Response: 177506
Conc: 1.46 ug/ml