

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010815.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 16:30
Operator : AJ\MA
Sample : PB145743BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB145743BL

Integration File: autoint1.e
Quant Time: Jun 23 01:10:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.820	2109425	18.662 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010815.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 16:30
Operator : AJ\MA
Sample : PB145743BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB145743BL

Integration File: autoint1.e
Quant Time: Jun 23 01:10:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

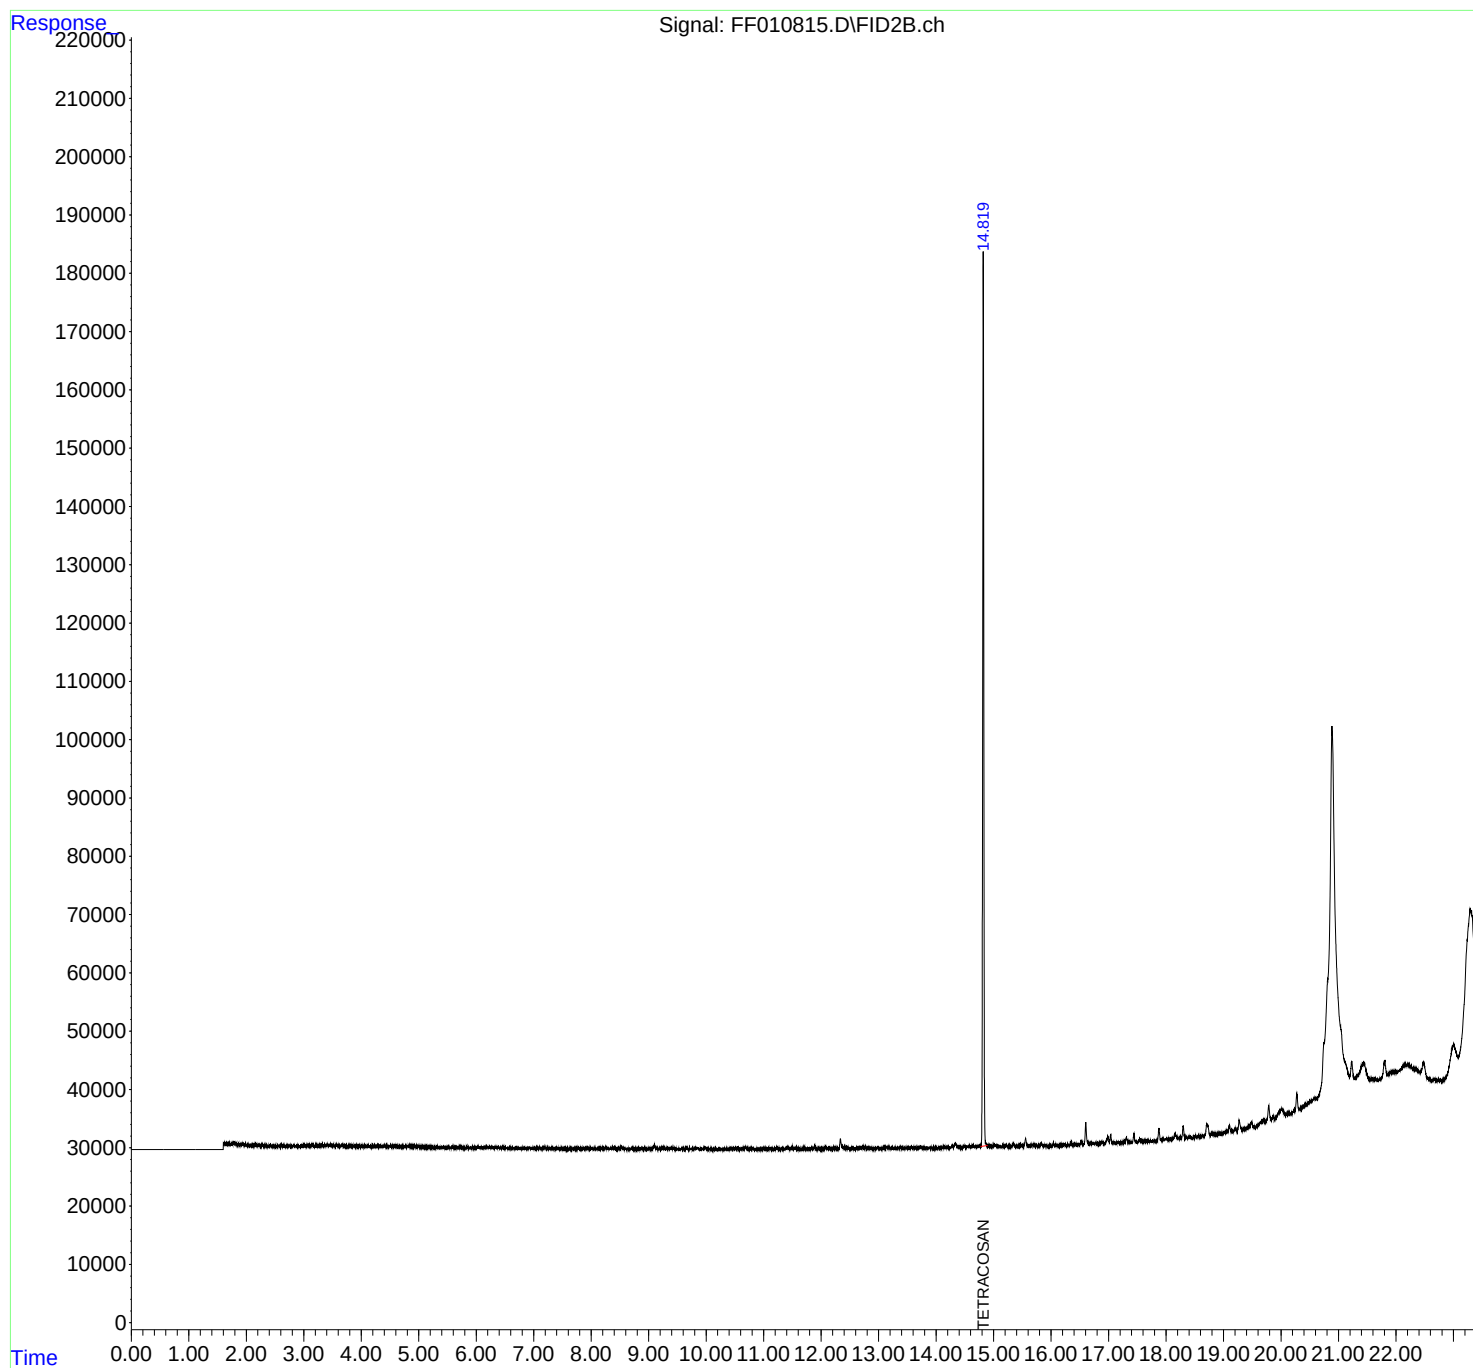

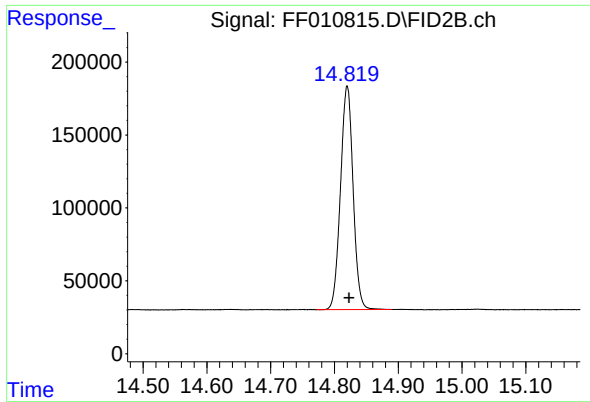

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.820 min
Delta R.T.: -0.003 min
Response: 2109425
Conc: 18.66 ug/ml

Instrument :
FID_F
ClientSampleId :
PB145743BL