

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010817.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 17:29
Operator : AJ\MA
Sample : N3422-05
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-12-GR

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

Integration File: autoint1.e
Quant Time: Jun 23 01:12:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.800	774659	6.853 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062222\
Data File : FF010817.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2022 17:29
Operator : AJ\MA
Sample : N3422-05
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
WC-14A-1A-12-GR


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

Integration File: autoint1.e
Quant Time: Jun 23 01:12:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

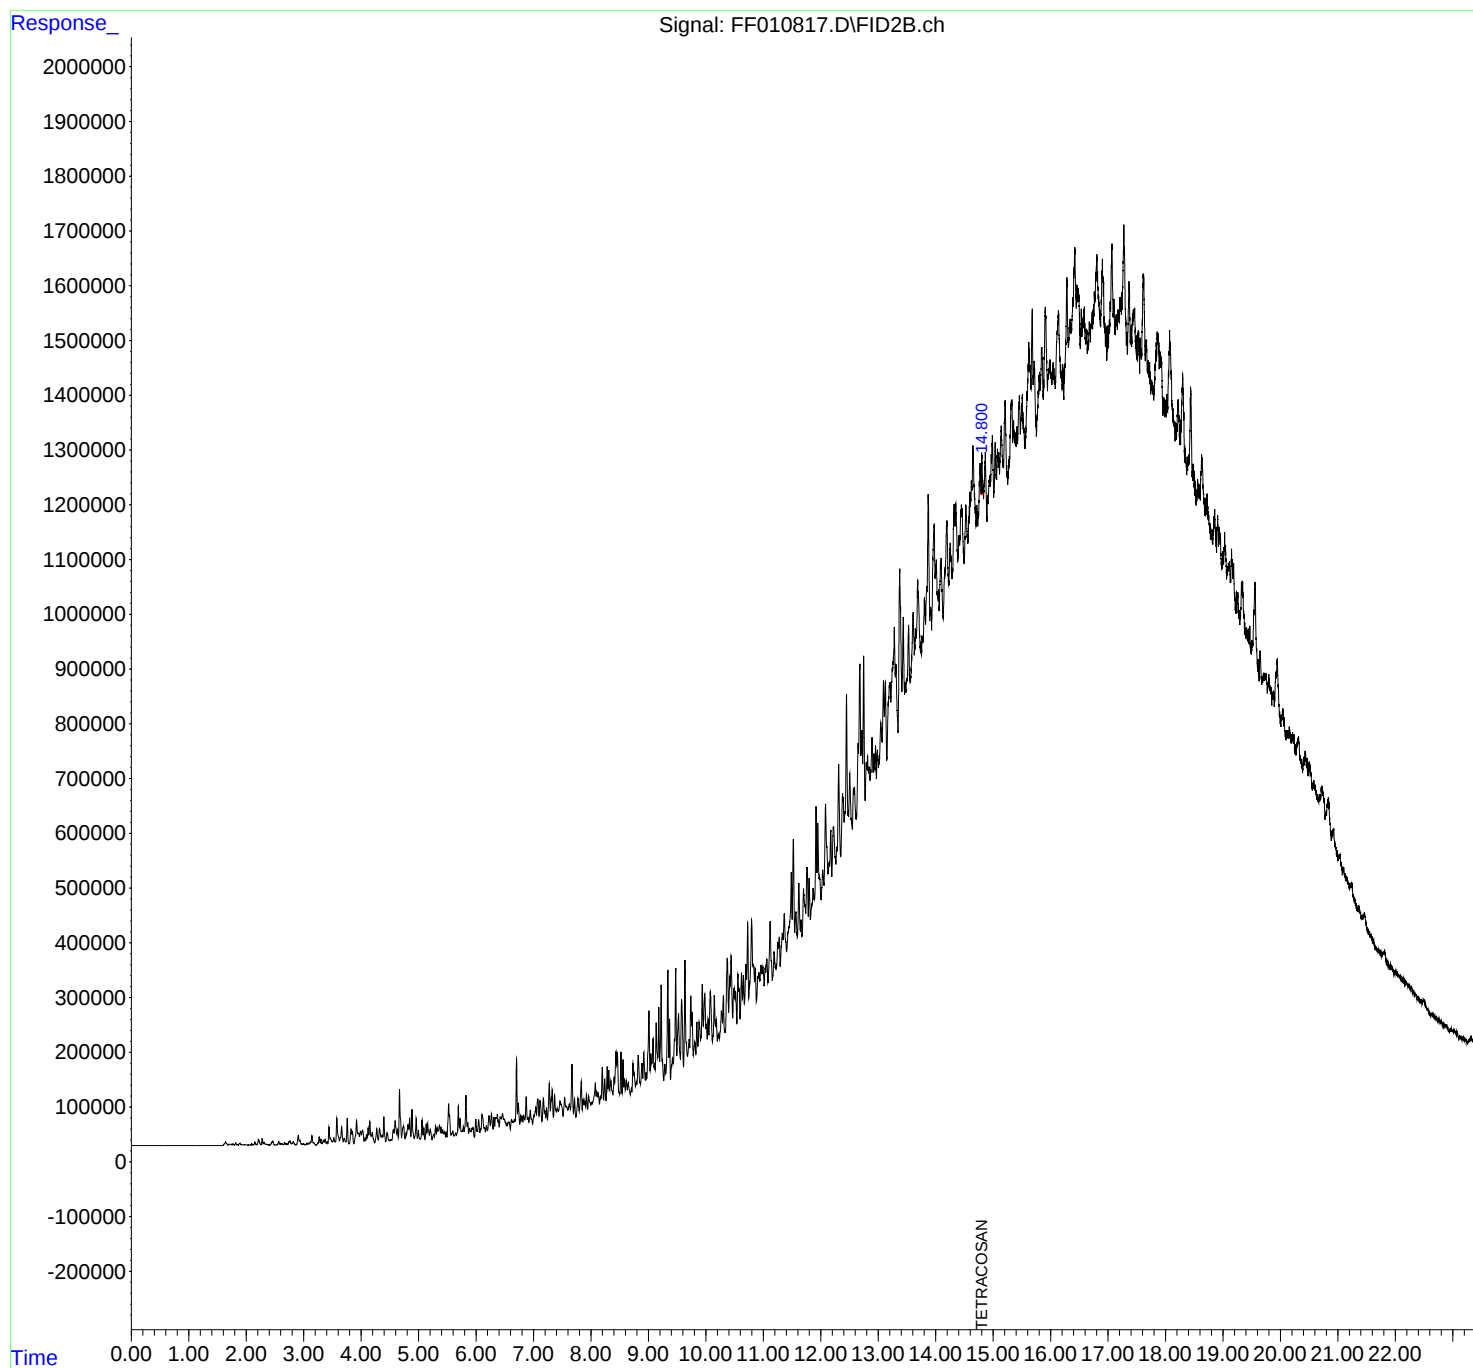

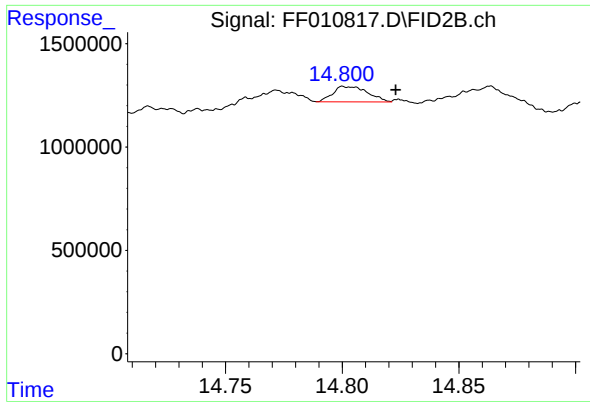

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.800 min
Delta R.T.: -0.023 min
Response: 774659
Conc: 6.85 ug/ml

Instrument :

FID_F

ClientSampleId :

WC-14A-1A-12-GR

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022