

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
 Data File : FF012933.D
 Signal(s) : FID2B.ch
 Acq On : 22 Jun 2023 13:10
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 23 01:42:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.689	2120908	16.274 ug/ml
12) N-OCTACOSANE	17.123	2262306	17.652 ug/ml
13) N-TRIACONTANE	18.007	212564	1.648 ug/ml
14) N-DOTRIACONTANE	18.837	291315	2.305 ug/ml
15) N-TETRATRIACONTANE	19.617	246895	2.078 ug/ml
16) N-HEXATRIACONTANE	20.358	189008	1.574 ug/ml
17) N-OCTATRIACONTANE	21.083f	209257	1.799 ug/ml
18) N-TETRACONTANE	21.967f	290367	2.334 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
Data File : FF012933.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2023 13:10
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 01:42:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

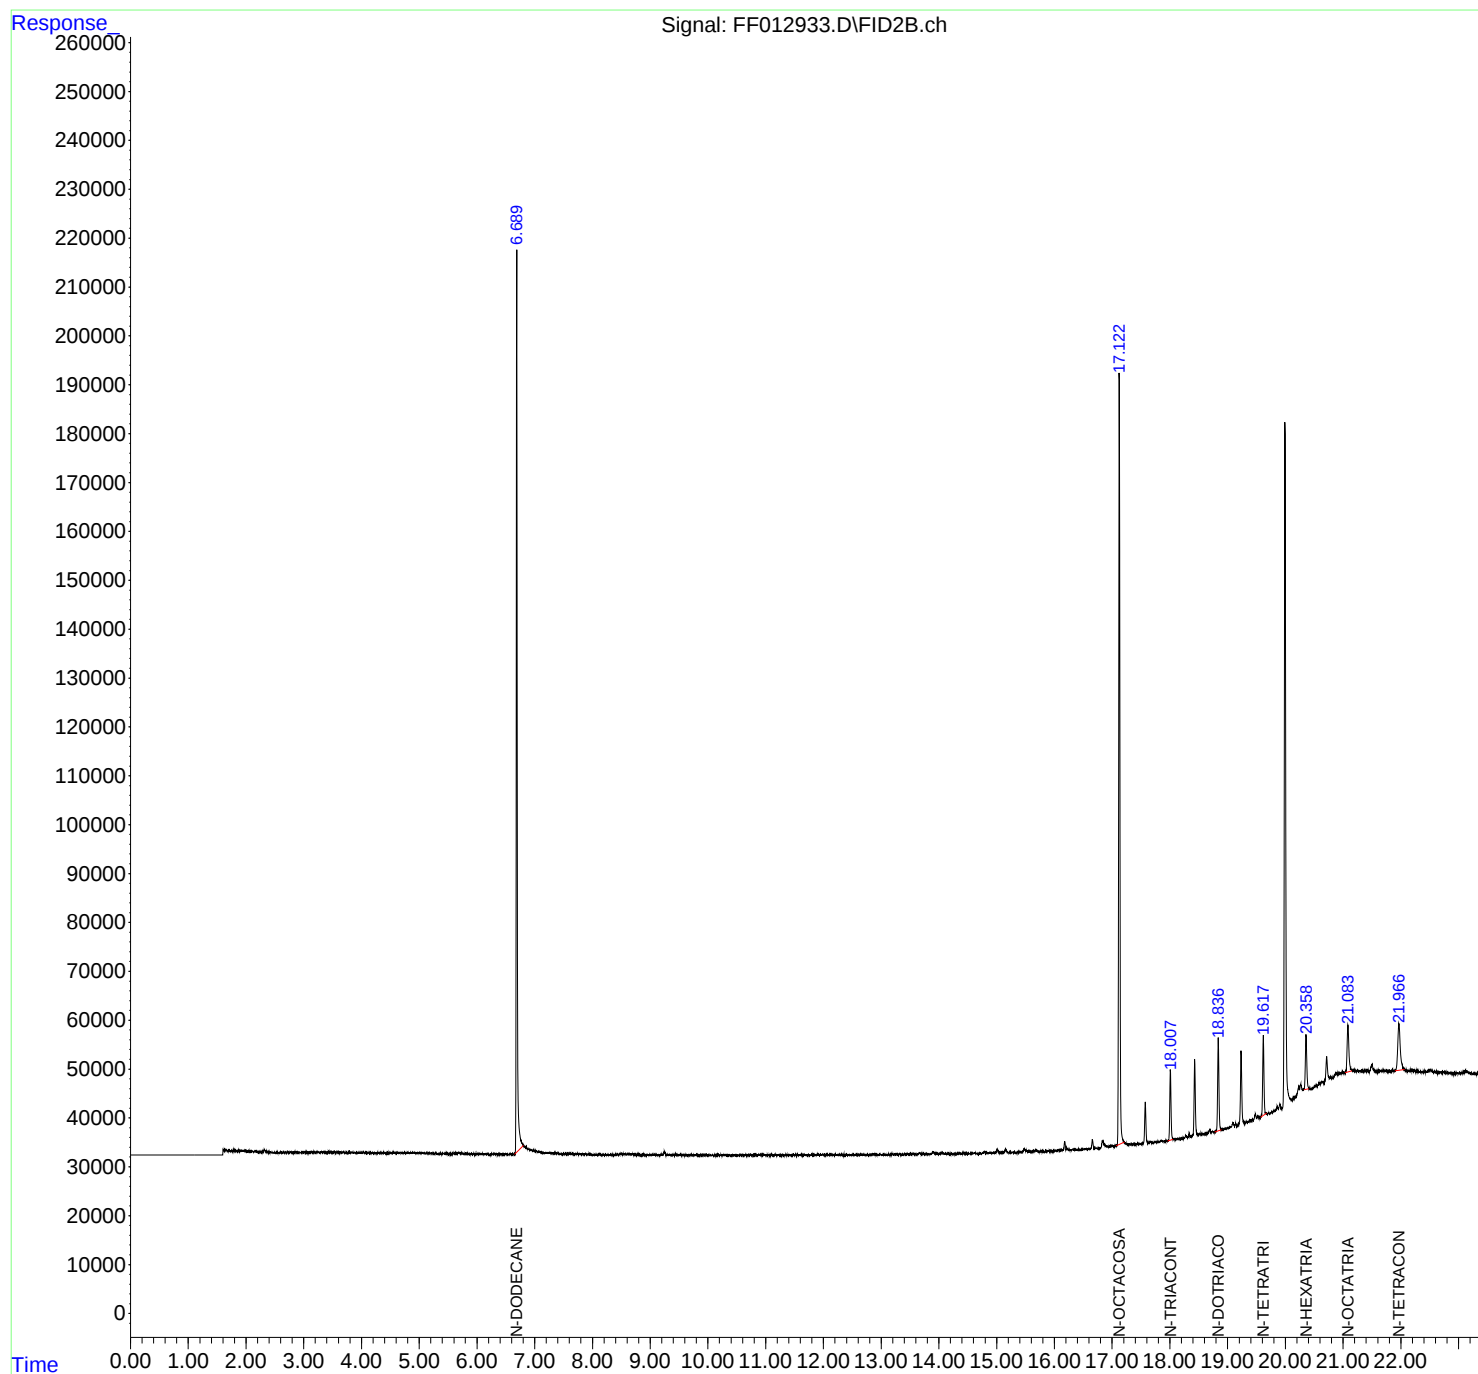

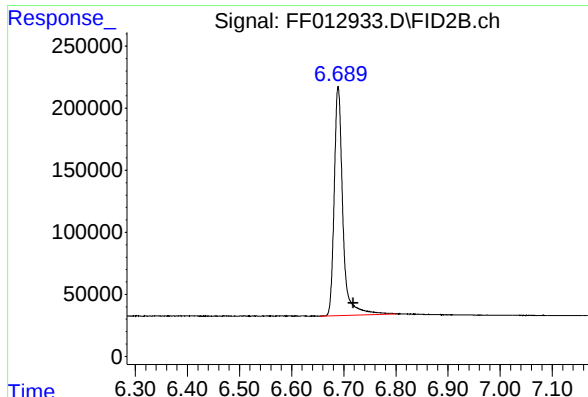


#3 N-DODECANE

R.T.: 6.689 min
Delta R.T.: -0.029 min
Response: 2120908
Conc: 16.27 ug/ml

Instrument :


FID_F

ClientSampleId :

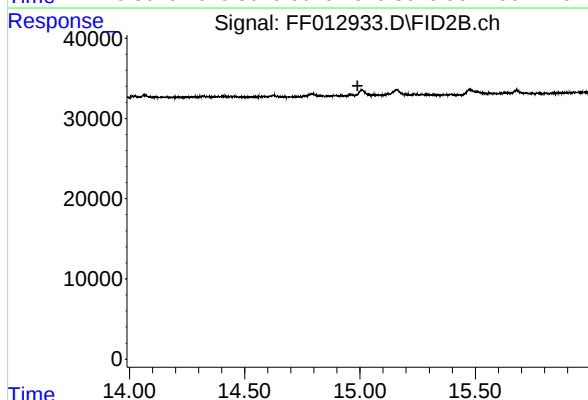


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.989 min
Response: 0
Conc: N.D.

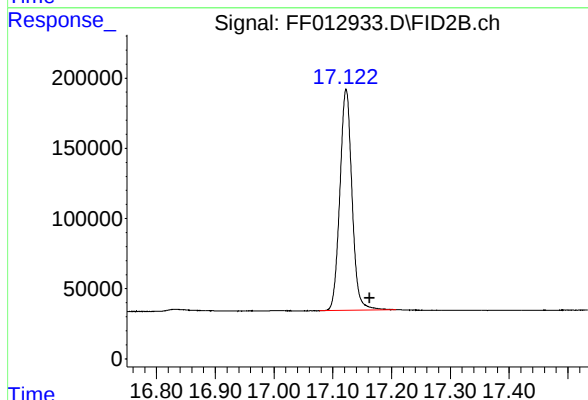


#12 N-OCTACOSANE

R.T.: 17.123 min
Delta R.T.: -0.040 min
Response: 2262306
Conc: 17.65 ug/ml

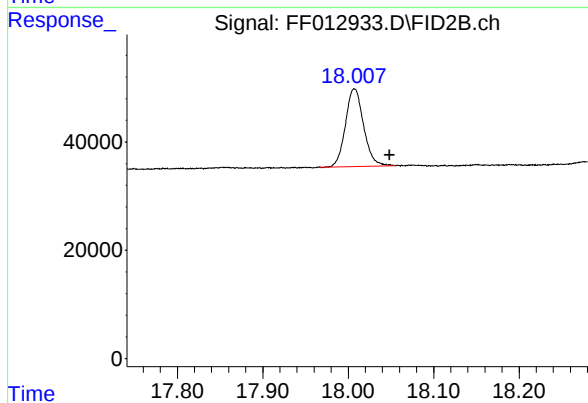

#13 N-TRIACONTANE


R.T.: 18.007 min
Delta R.T.: -0.041 min
Response: 212564
Conc: 1.65 ug/ml

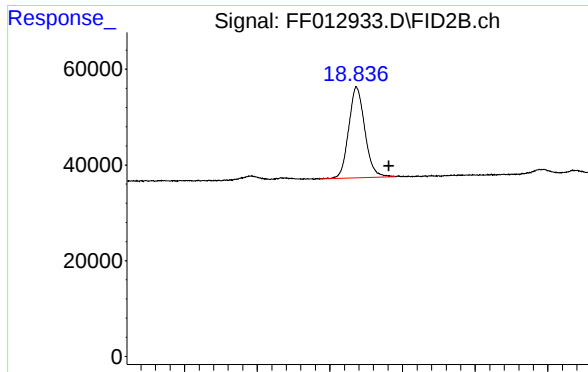

#14 N-DOTRIACONTANE


R.T.: 18.837 min
Delta R.T.: -0.045 min
Response: 291315
Conc: 2.30 ug/ml

Instrument :
FID_F
ClientSampleId :

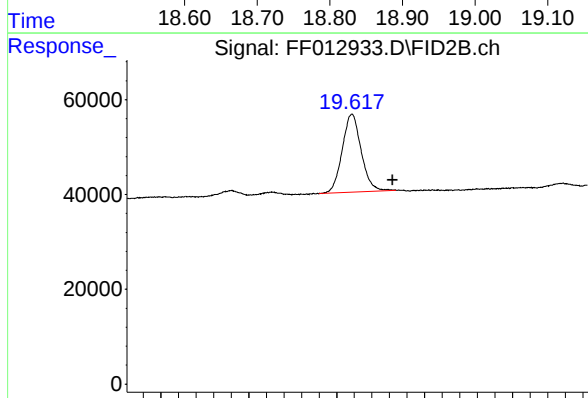


#15 N-TETRATRIACONTANE

R.T.: 19.617 min
Delta R.T.: -0.046 min
Response: 246895
Conc: 2.08 ug/ml

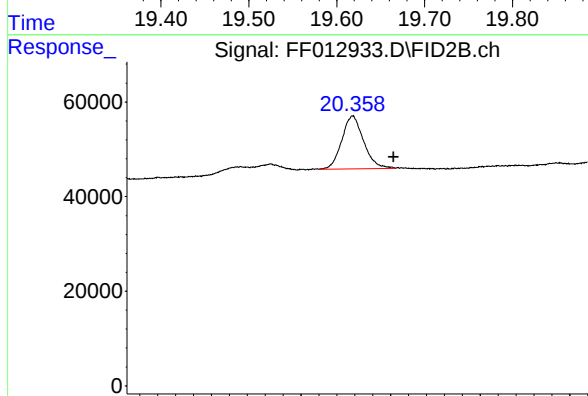


#16 N-HEXATRIACONTANE

R.T.: 20.358 min
Delta R.T.: -0.045 min
Response: 189008
Conc: 1.57 ug/ml

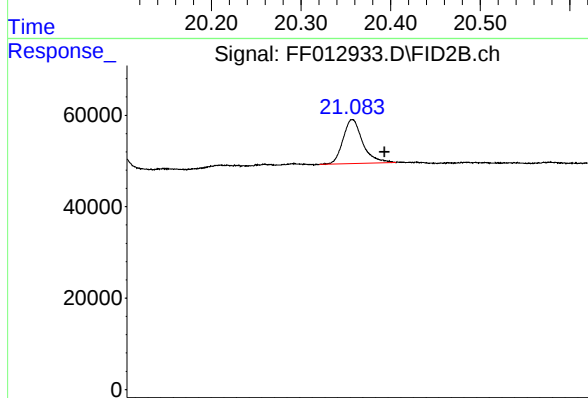

#17 N-OCTATRIACONTANE

R.T.: 21.083 min
Delta R.T.: -0.051 min
Response: 209257
Conc: 1.80 ug/ml

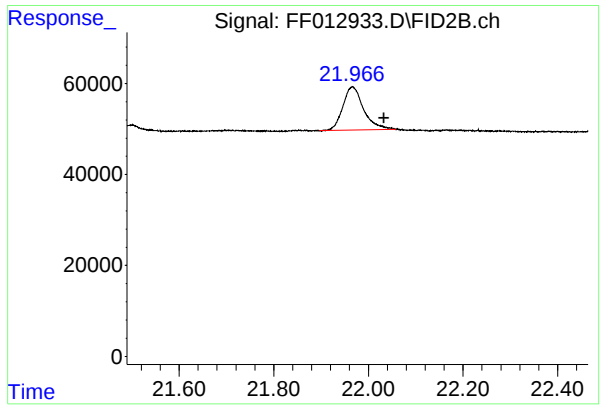

#18 N-TETRACONTANE

R.T.: 21.967 min
Delta R.T.: -0.067 min
Response: 290367
Conc: 2.33 ug/ml

Instrument :
FID_F
ClientSampleId :