

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
 Data File : FF012956.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 06:00
 Operator : YP\AJ
 Sample : 03366-04
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 23 06:21:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.956	1377820	11.799 ug/ml
Target Compounds			
7) N-EICOSANE	12.943	759971	5.549 ug/ml
10) N-TETRACOSANE	15.166	515835	3.903 ug/ml
11) N-HEXACOSANE	16.178	96108	0.744 ug/ml
12) N-OCTACOSANE	17.122	168585	1.315 ug/ml
13) N-TRIACONTANE	18.011	117650	0.912 ug/ml
14) N-DOTRIACONTANE	18.836	365133	2.889 ug/ml
15) N-TETRATRIACONTANE	19.697	77827	0.655 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
Data File : FF012956.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 06:00
Operator : YP\AJ
Sample : 03366-04
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 06:21:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

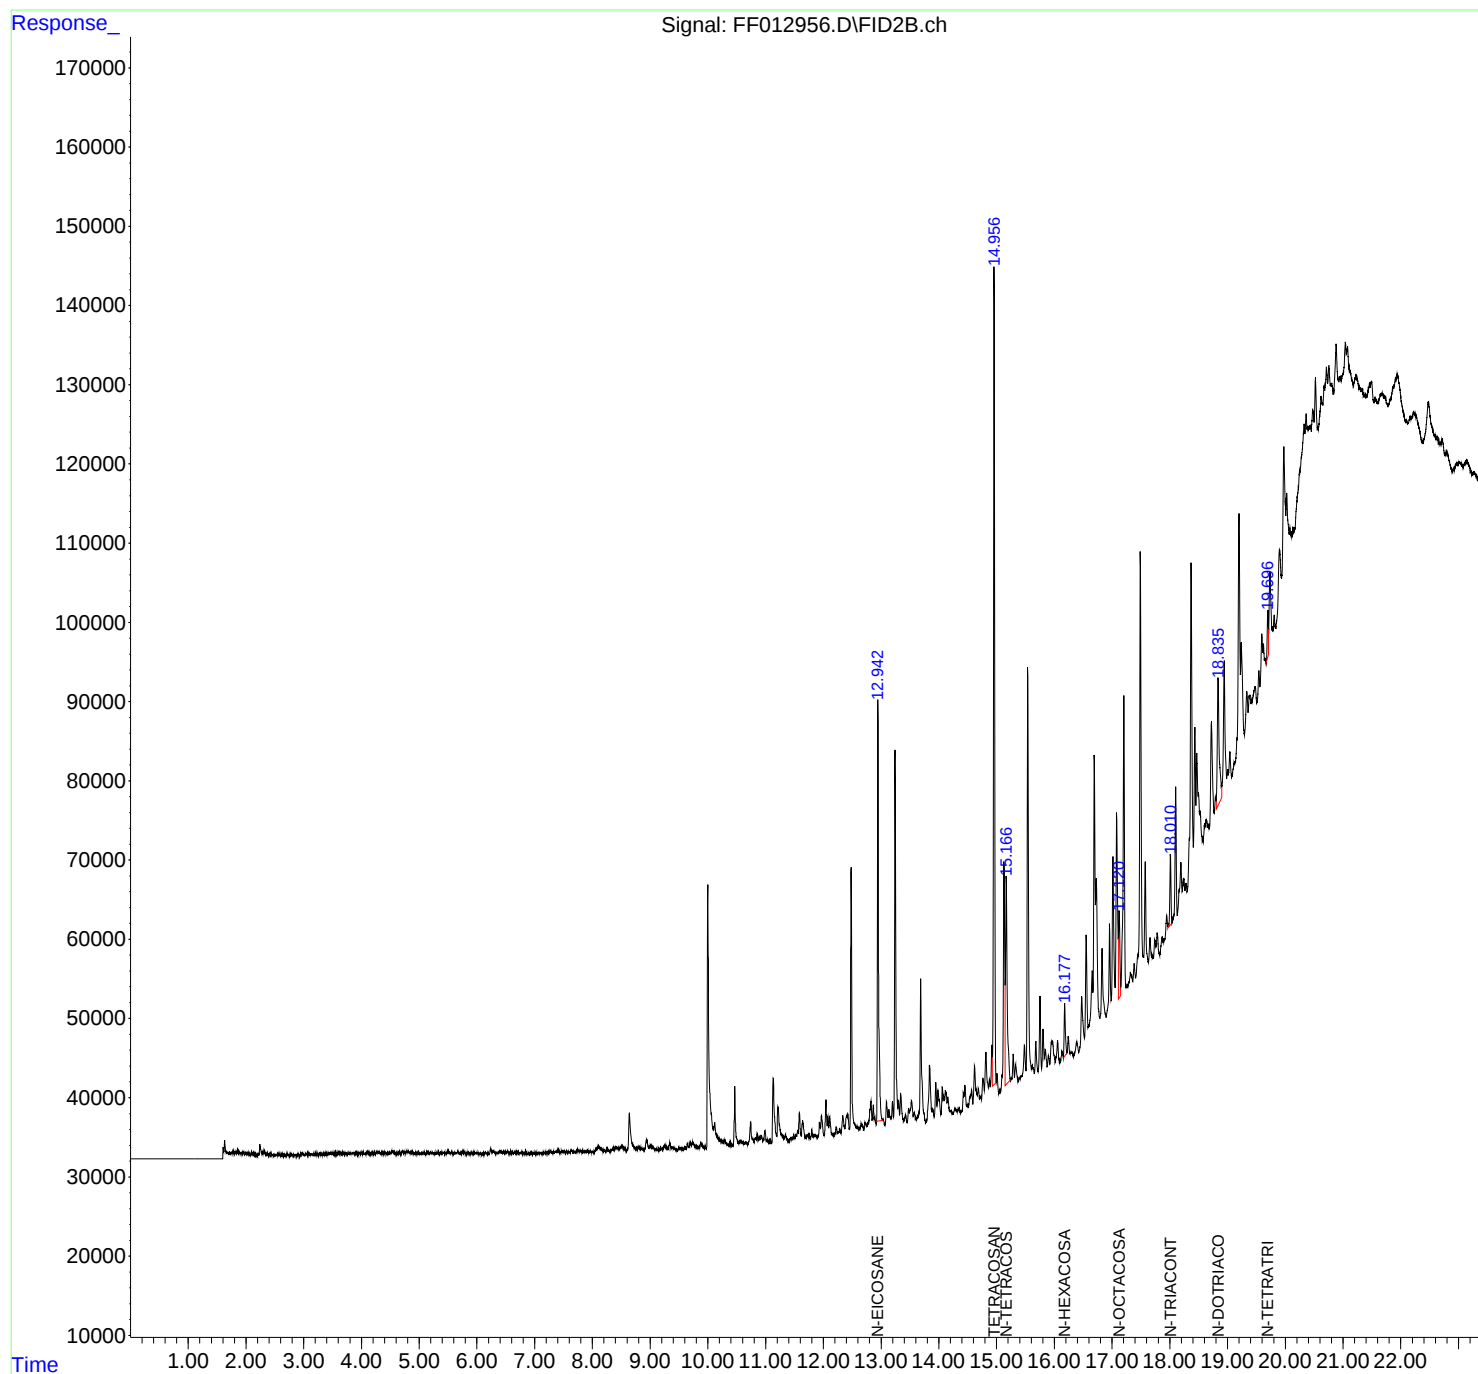


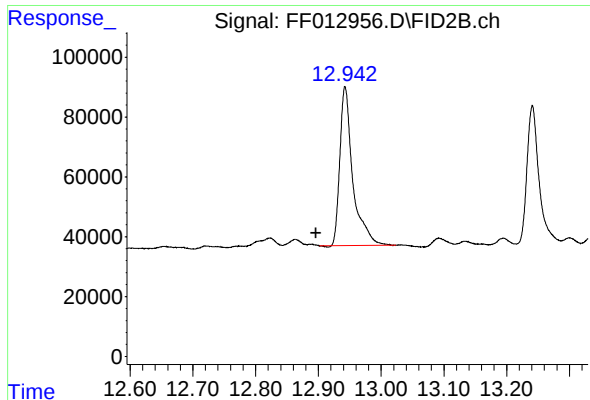

#7 N-EICOSANE


R.T.: 12.943 min
Delta R.T.: 0.046 min
Response: 759971
Conc: 5.55 ug/ml

Instrument :
FID_F
ClientSampleId :

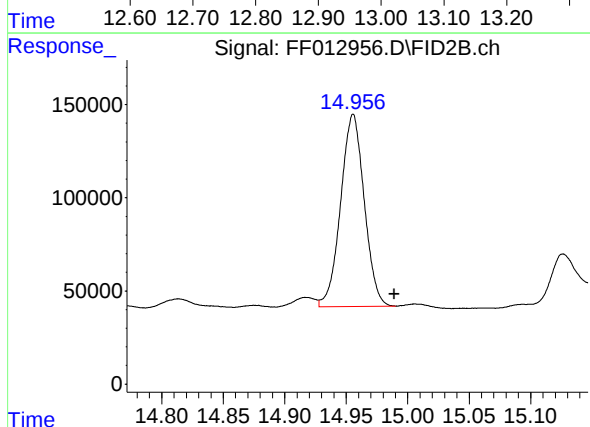


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.956 min
Delta R.T.: -0.033 min
Response: 1377820
Conc: 11.80 ug/ml

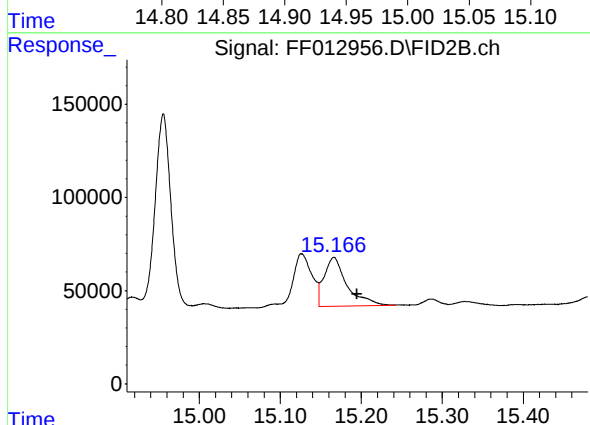


#10 N-TETRACOSANE

R.T.: 15.166 min
Delta R.T.: -0.028 min
Response: 515835
Conc: 3.90 ug/ml

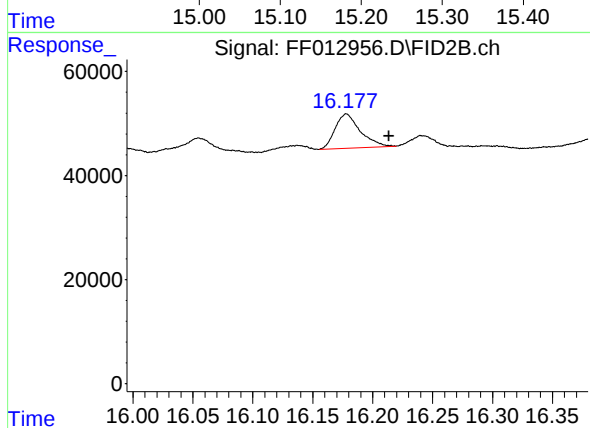

#11 N-HEXACOSANE


R.T.: 16.178 min
Delta R.T.: -0.035 min
Response: 96108
Conc: 0.74 ug/ml

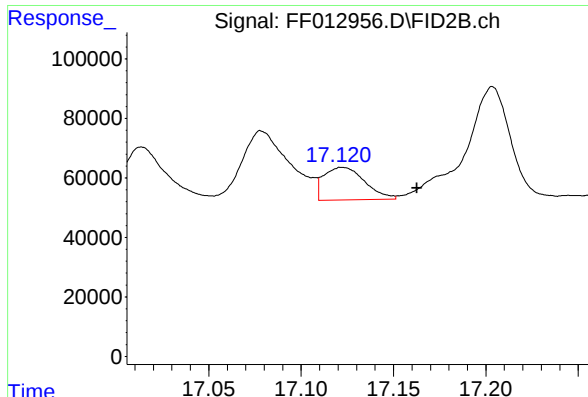

#12 N-OCTACOSANE


R.T.: 17.122 min
Delta R.T.: -0.040 min
Response: 168585
Conc: 1.32 ug/ml

Instrument :
FID_F
ClientSampleId :

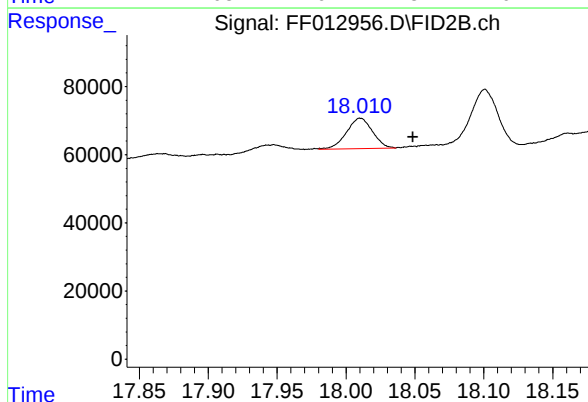


#13 N-TRIACONTANE

R.T.: 18.011 min
Delta R.T.: -0.038 min
Response: 117650
Conc: 0.91 ug/ml

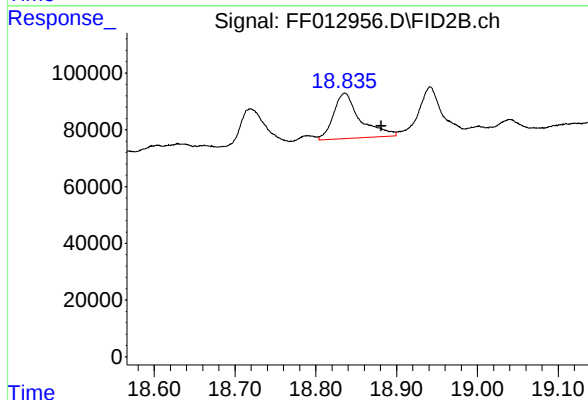

#14 N-DOTRIACONTANE

R.T.: 18.836 min
Delta R.T.: -0.045 min
Response: 365133
Conc: 2.89 ug/ml

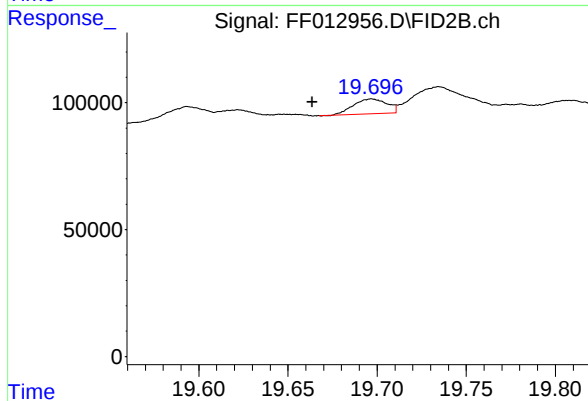

#15 N-TETRATRIACONTANE

R.T.: 19.697 min
Delta R.T.: 0.033 min
Response: 77827
Conc: 0.66 ug/ml