

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
Data File : FF012941.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2023 21:13
Operator : YP\AJ
Sample : 03355-08
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-04-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

Integration File: autoint1.e
Quant Time: Jun 23 01:43:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.962	1339528	11.471 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
Data File : FF012941.D
Signal(s) : FID2B.ch
Acq On : 22 Jun 2023 21:13
Operator : YP\AJ
Sample : 03355-08
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SB-04-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

Integration File: autoint1.e
Quant Time: Jun 23 01:43:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

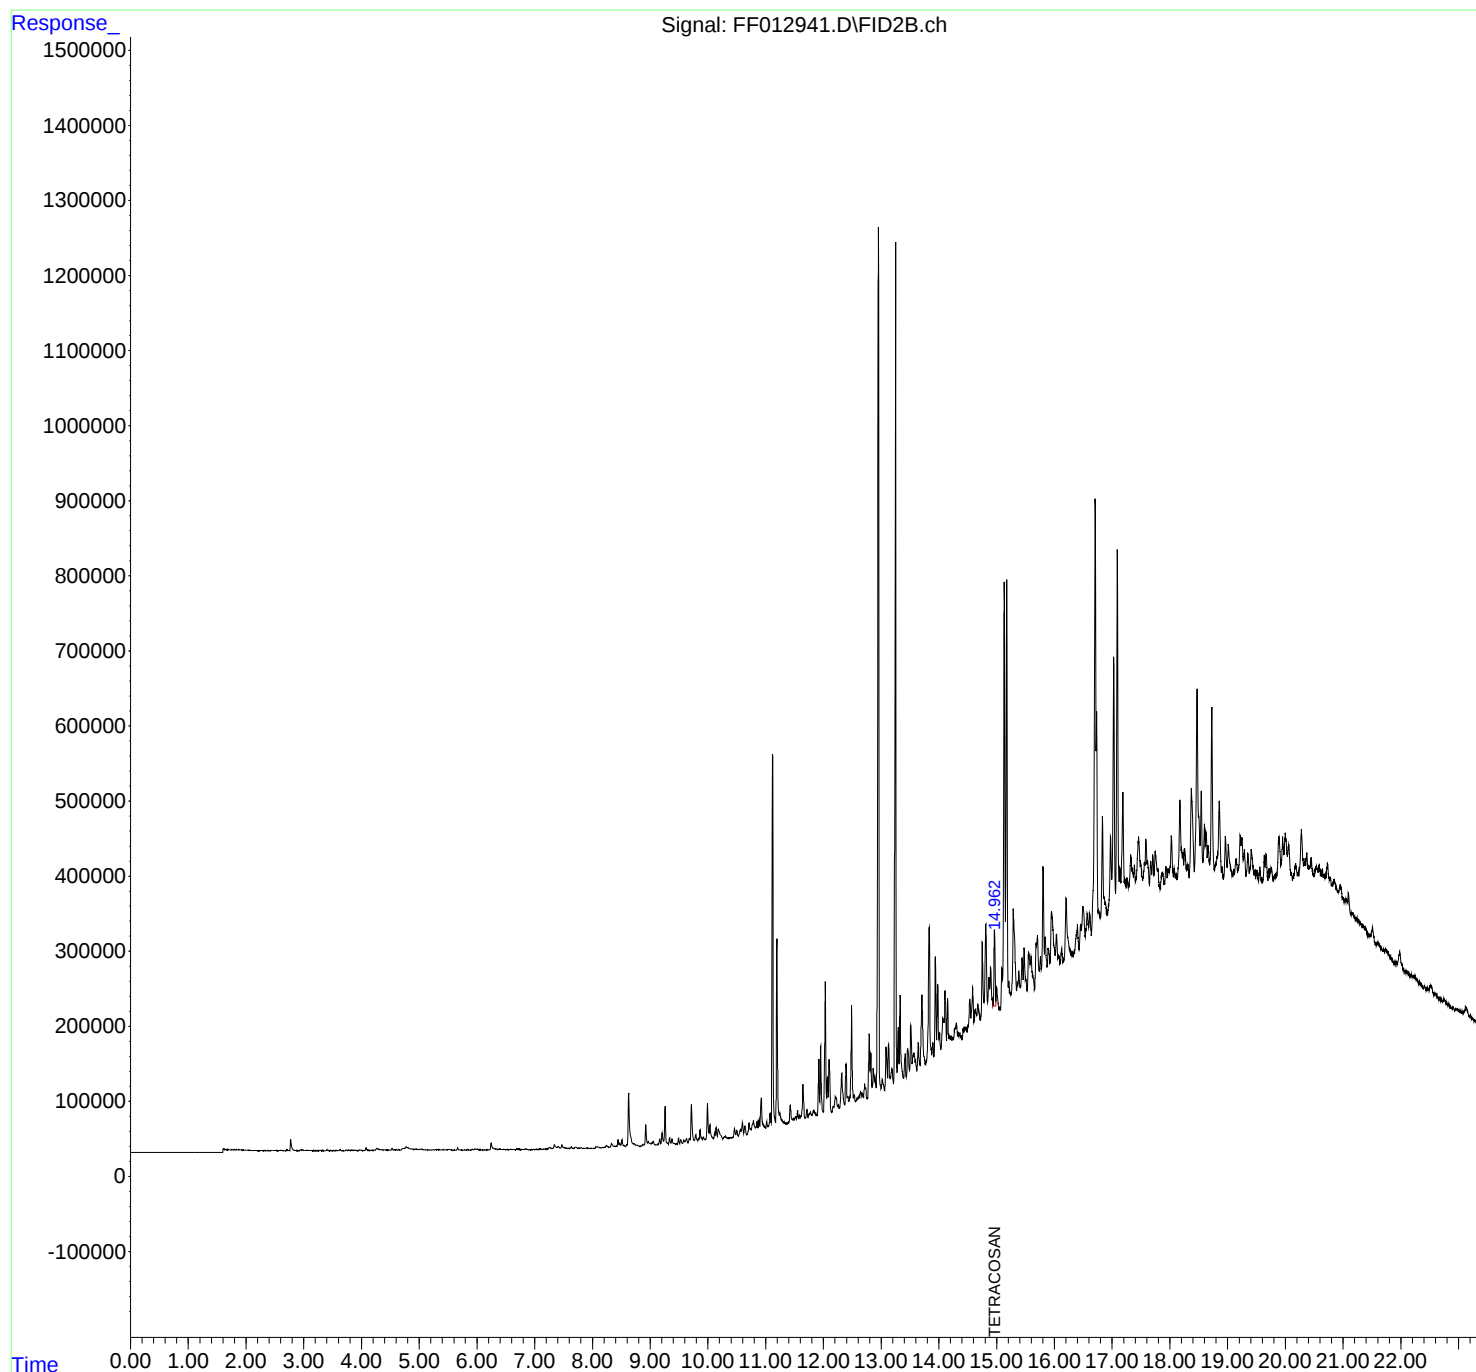

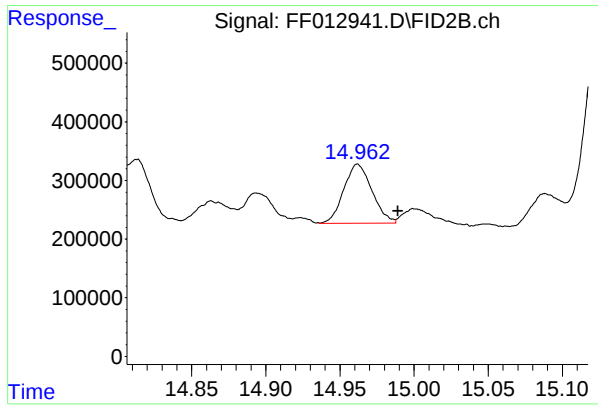

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.962 min
Delta R.T.: -0.027 min
Response: 1339528
Conc: 11.47 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-04-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023