

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
Data File : FF012954.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 05:01
Operator : YP\AJ
Sample : 03360-07
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CE-88N-062023

Integration File: autoint1.e
Quant Time: Jun 23 06:05:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.957	2265825	19.403 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062223\
Data File : FF012954.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 05:01
Operator : YP\AJ
Sample : 03360-07
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CE-88N-062023

Integration File: autoint1.e
Quant Time: Jun 23 06:05:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

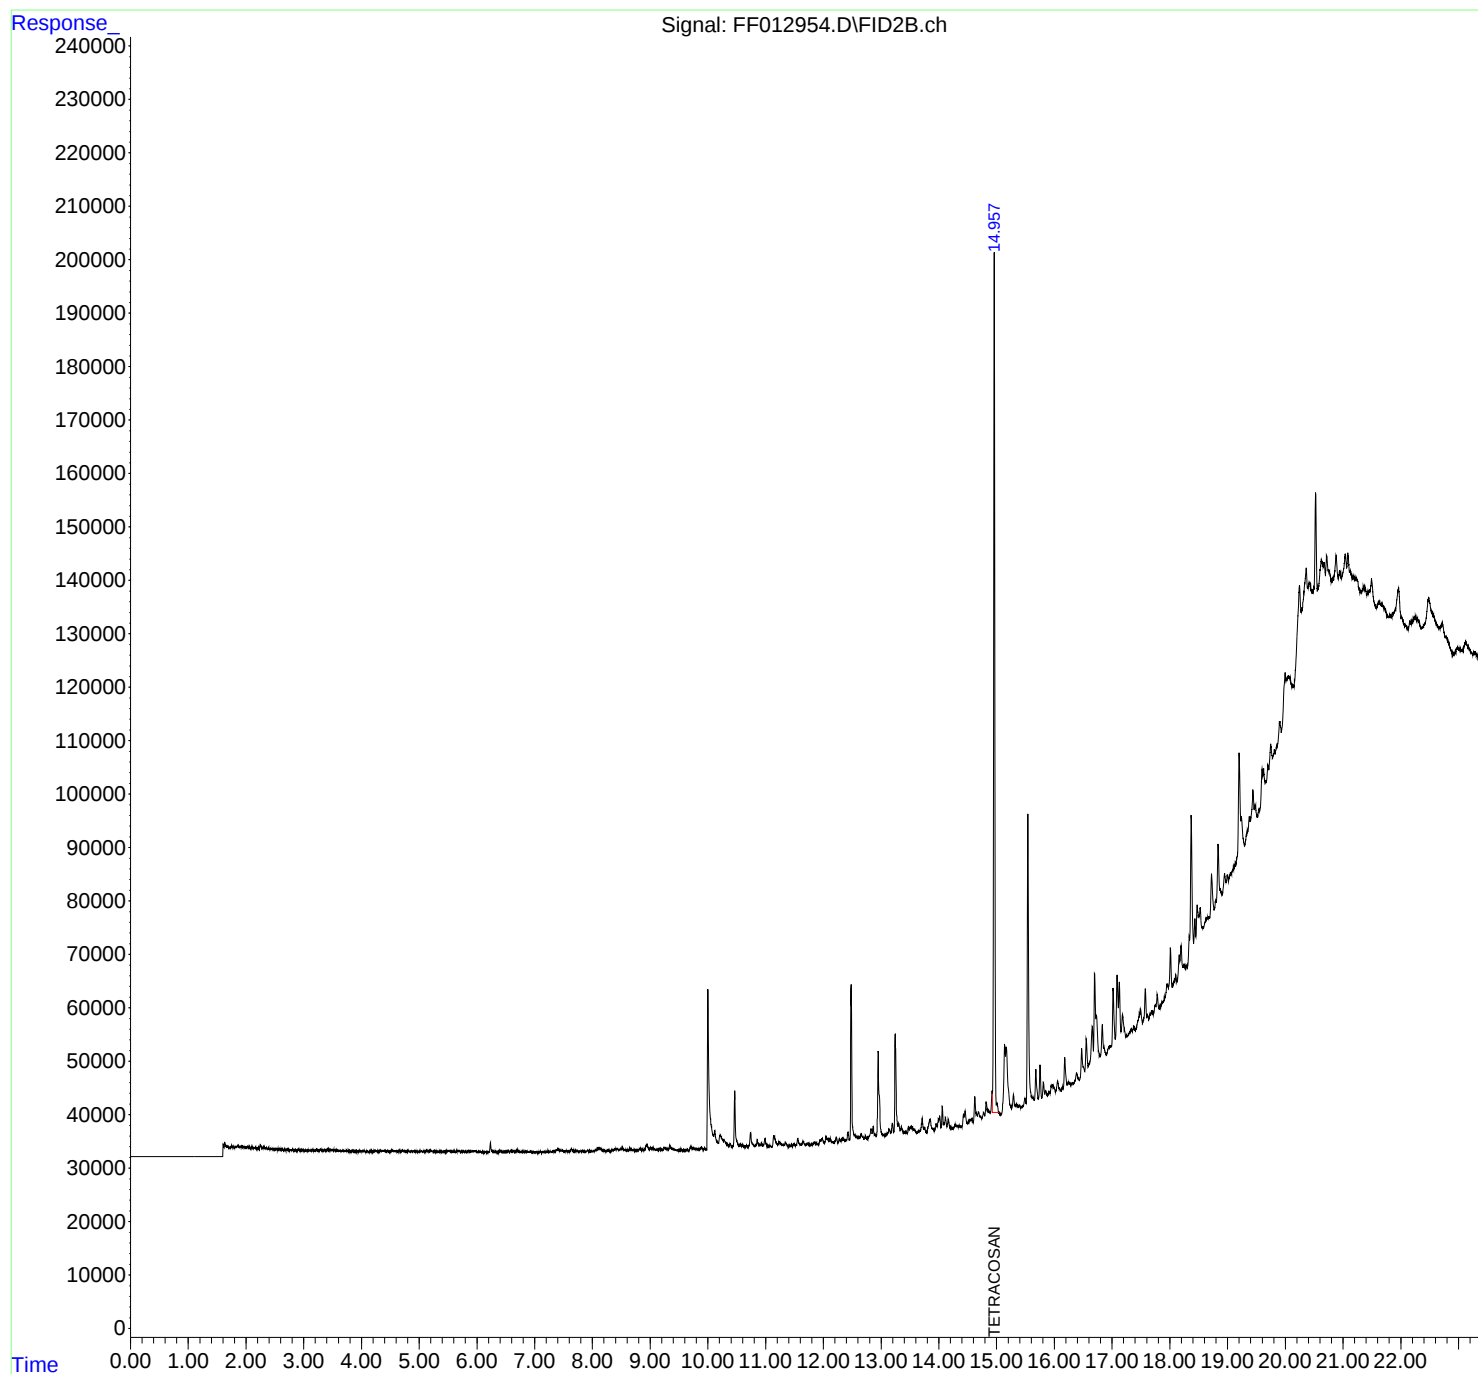

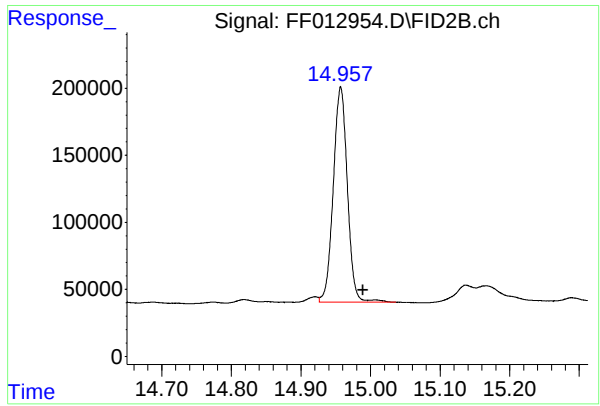

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.957 min
Delta R.T.: -0.032 min
Response: 2265825
Conc: 19.40 ug/ml

Instrument :
FID_F
ClientSampleId :
CE-88N-062023