

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
 Data File : FF001072.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2018 12:18
 Operator : UA\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 02:14:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.348	1494227	11.153 ug/ml
8) N-DOCOSANE	13.568	1419067	10.732 ug/ml
10) N-TETRACOSANE	14.674	897359	6.918 ug/ml
11) N-HEXACOSANE	15.695	826065	6.431 ug/ml
12) N-OCTACOSANE	16.646	597060	4.695 ug/ml
13) N-TRIACONTANE	17.534	561986	4.451 ug/ml
14) N-DOTRIACONTANE	18.364	876820	7.149 ug/ml
15) N-TETRATRIACONTANE	19.154	482765	4.023 ug/ml
16) N-HEXATRIACONTANE	19.899	401278	3.515 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
Data File : FF001072.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2018 12:18
Operator : UA\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 02:14:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

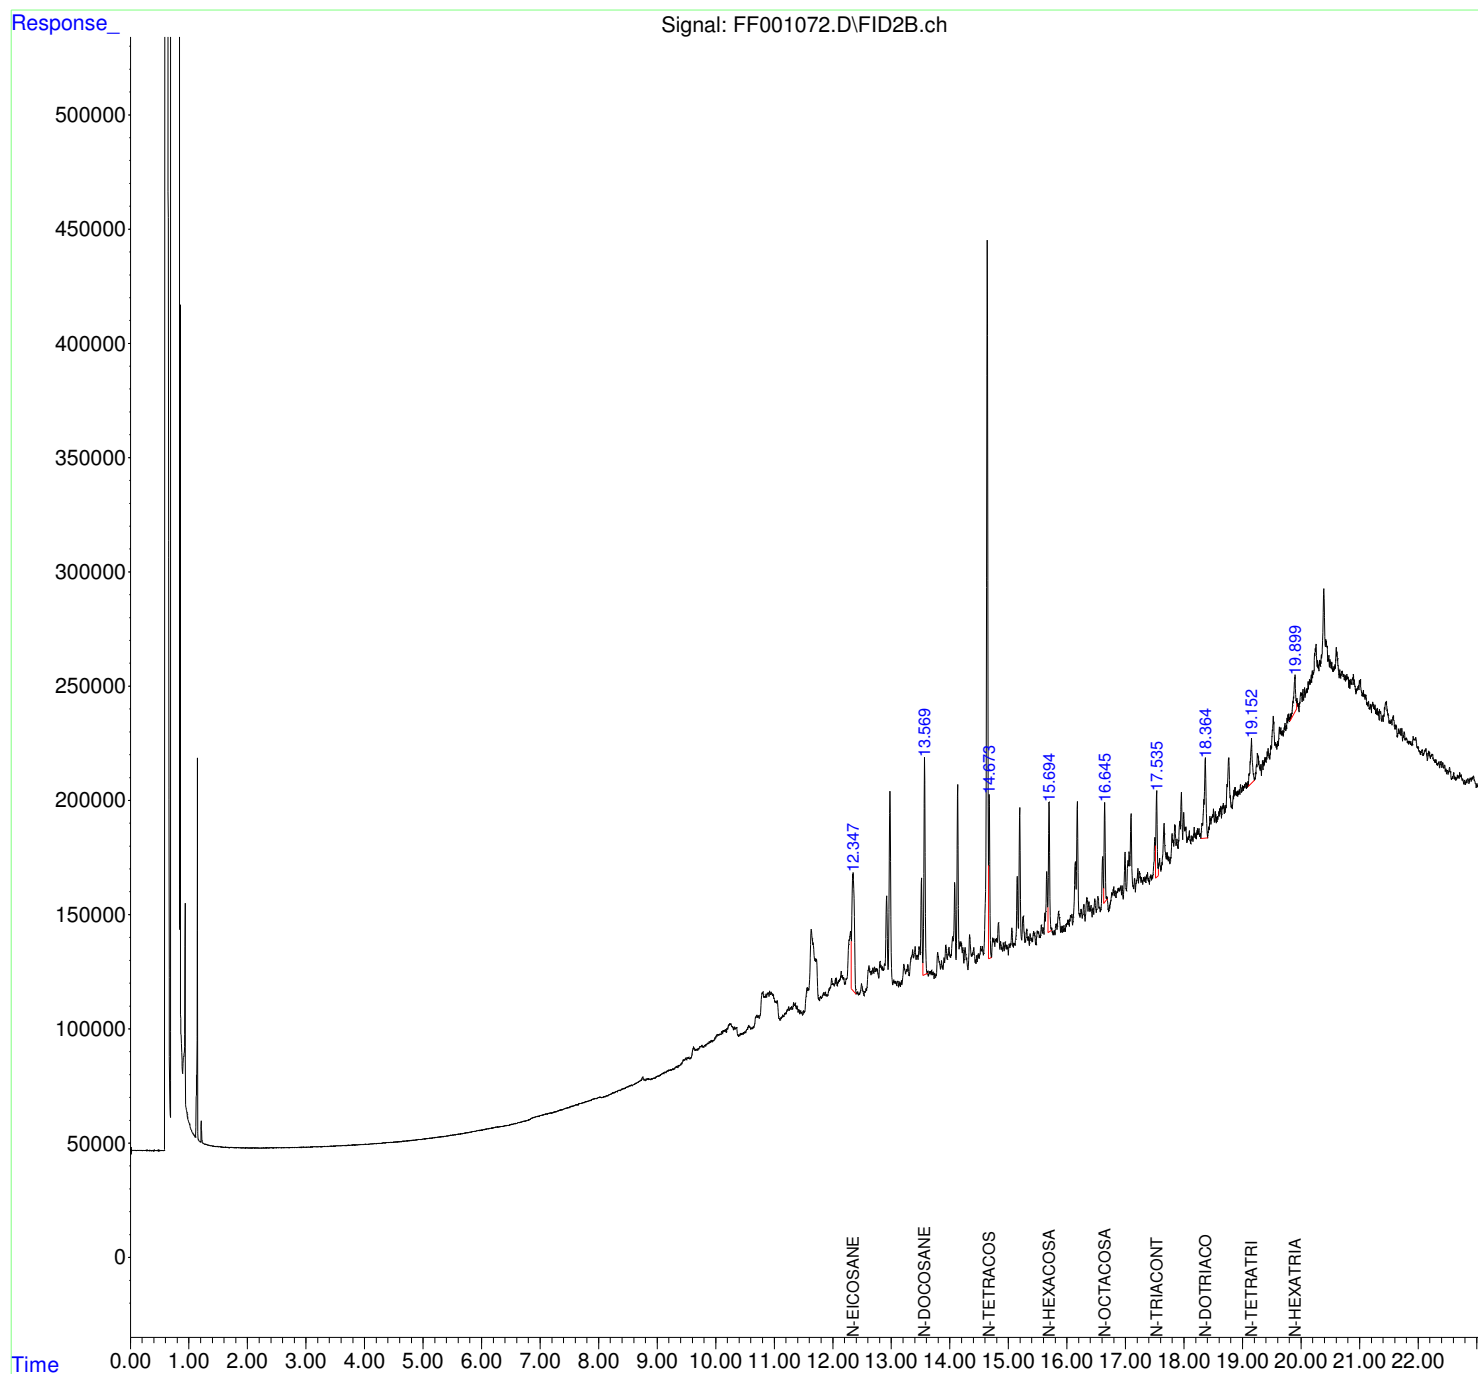


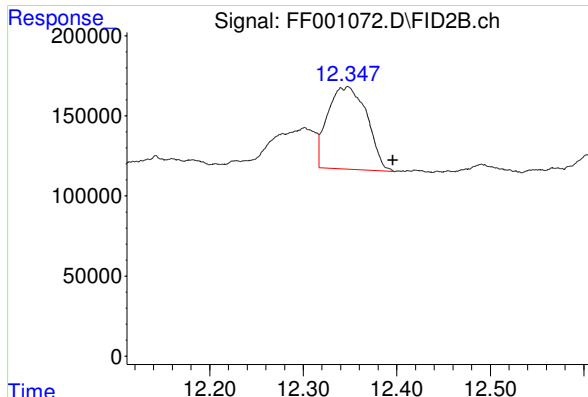

#7 N-EICOSANE


R.T.: 12.348 min
Delta R.T.: -0.048 min
Response: 1494227
Conc: 11.15 ug/ml

Instrument :
FID_F
ClientSampleId :

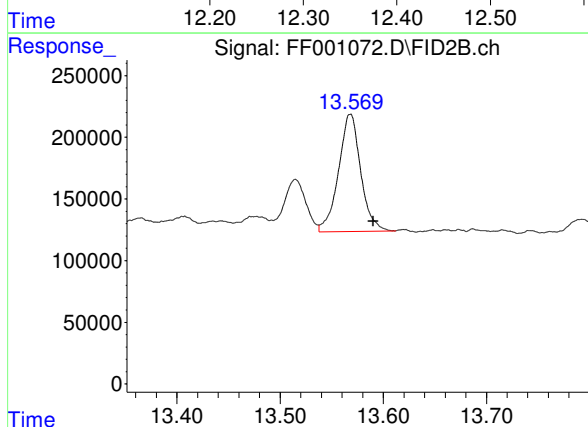


#8 N-DOCOSANE

R.T.: 13.568 min
Delta R.T.: -0.022 min
Response: 1419067
Conc: 10.73 ug/ml

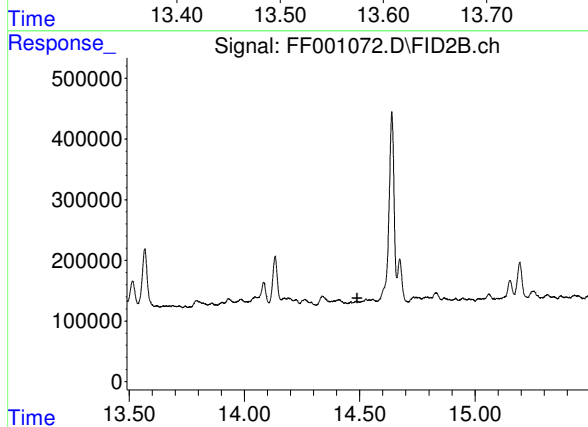


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.490 min
Response: 0
Conc: N.D.

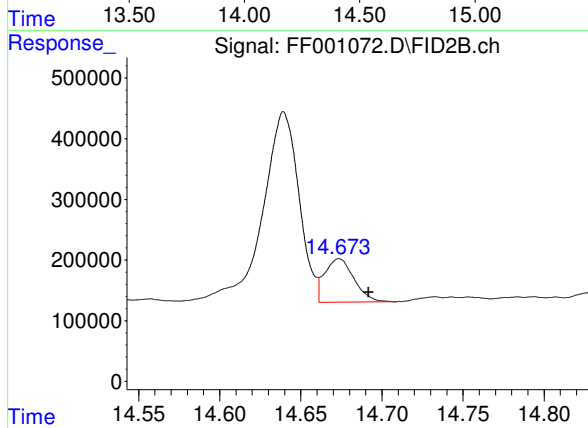

#10 N-TETRACOSANE


R.T.: 14.674 min
Delta R.T.: -0.018 min
Response: 897359
Conc: 6.92 ug/ml

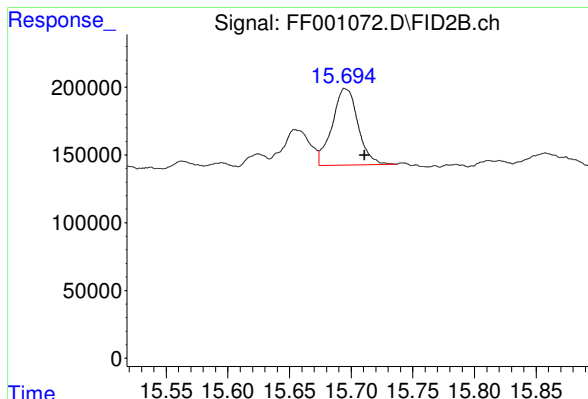

#11 N-HEXACOSANE


R.T.: 15.695 min
Delta R.T.: -0.015 min
Response: 826065
Conc: 6.43 ug/ml

Instrument :
FID_F
ClientSampleId :

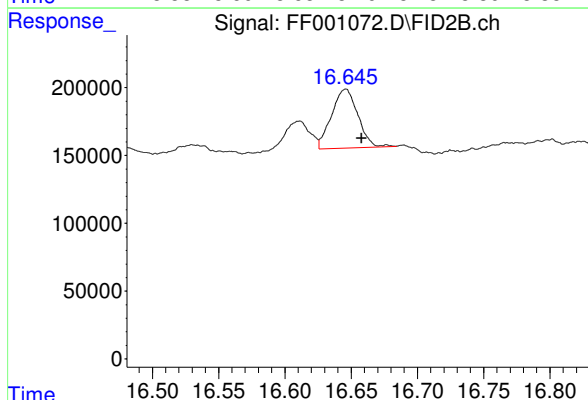


#12 N-OCTACOSANE

R.T.: 16.646 min
Delta R.T.: -0.012 min
Response: 597060
Conc: 4.70 ug/ml

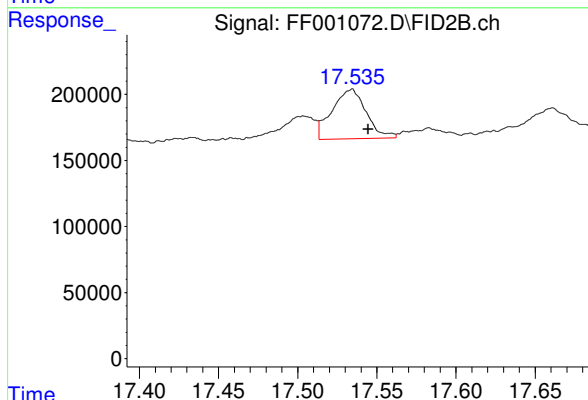


#13 N-TRIACONTANE

R.T.: 17.534 min
Delta R.T.: -0.011 min
Response: 561986
Conc: 4.45 ug/ml

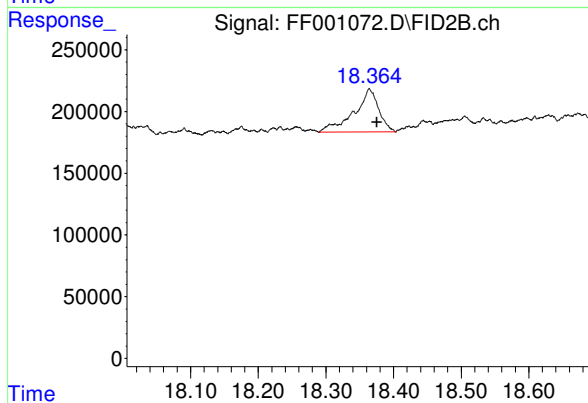

#14 N-DOTRIACONTANE


R.T.: 18.364 min
Delta R.T.: -0.011 min
Response: 876820
Conc: 7.15 ug/ml

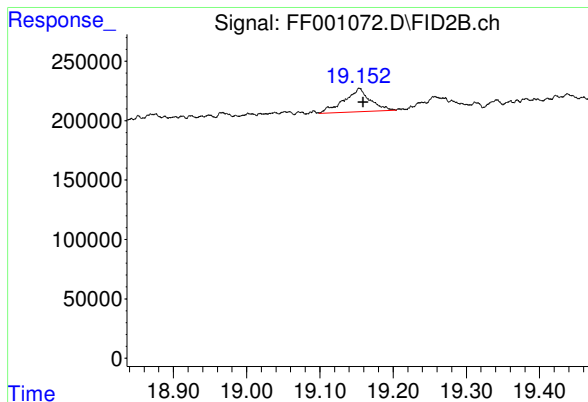

#15 N-TETRATRIACONTANE

R.T.: 19.154 min
Delta R.T.: -0.005 min
Response: 482765
Conc: 4.02 ug/ml

Instrument :
FID_F
ClientSampleId :

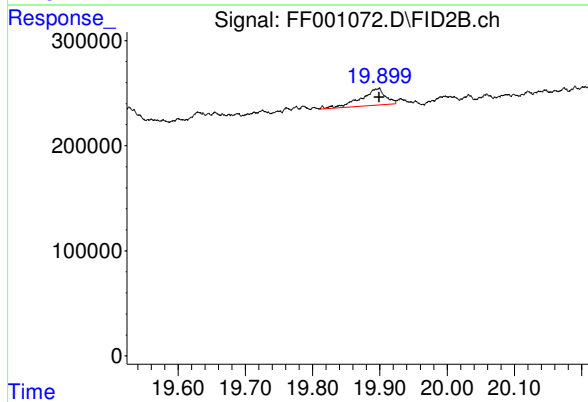

#16 N-HEXATRIACONTANE

R.T.: 19.899 min
Delta R.T.: 0.000 min
Response: 401278
Conc: 3.51 ug/ml