

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062318\  
Data File : FF001075.D  
Signal(s) : FID2B.ch  
Acq On : 23 Jun 2018 13:51  
Operator : UA\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 25 02:14:19 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF060118.M  
Quant Title :  
QLast Update : Fri Jun 01 16:01:51 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.250  | 2847954  | 20.320 ug/ml |
| 12)                         | N-OCTACOSANE | 16.651 | 2398198  | 18.860 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062318\  
Data File : FF001075.D  
Signal(s) : FID2B.ch  
Acq On : 23 Jun 2018 13:51  
Operator : UA\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 25 02:14:19 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID\_F\Method\FF060118.M  
Quant Title :  
QLast Update : Fri Jun 01 16:01:51 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

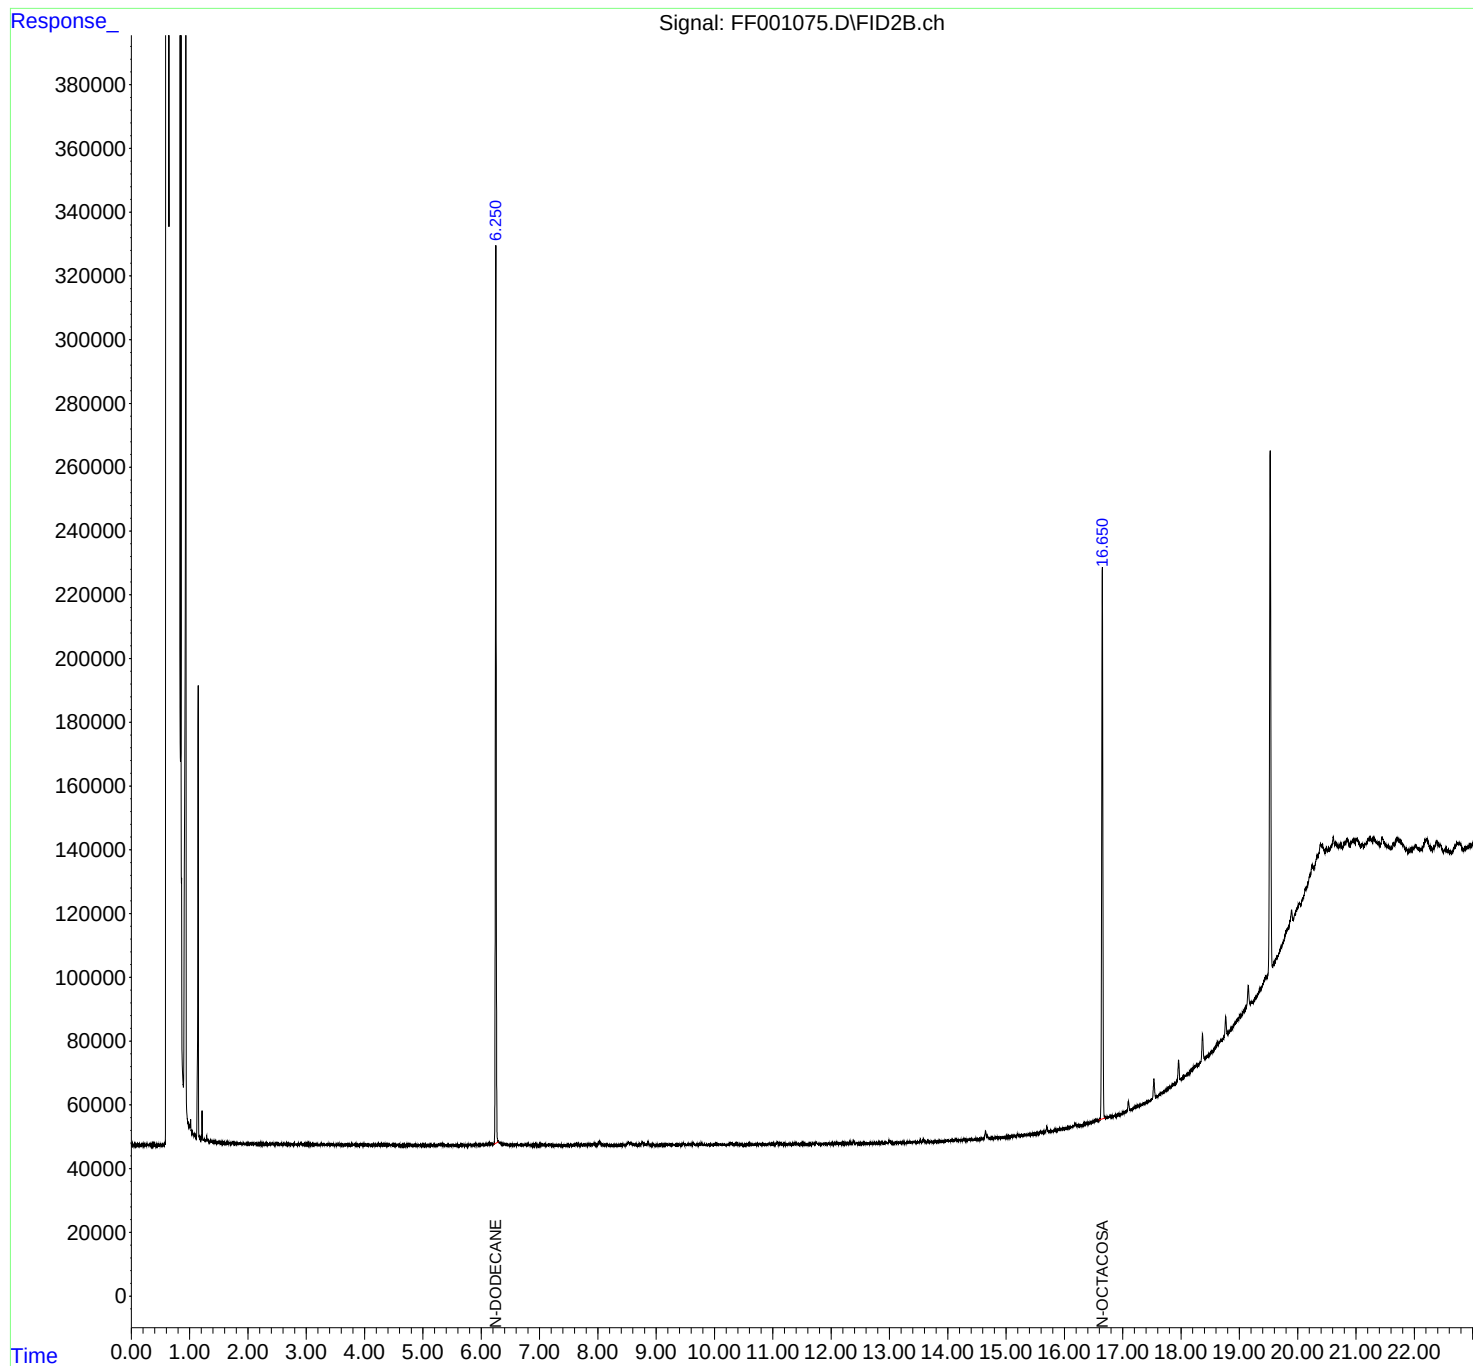


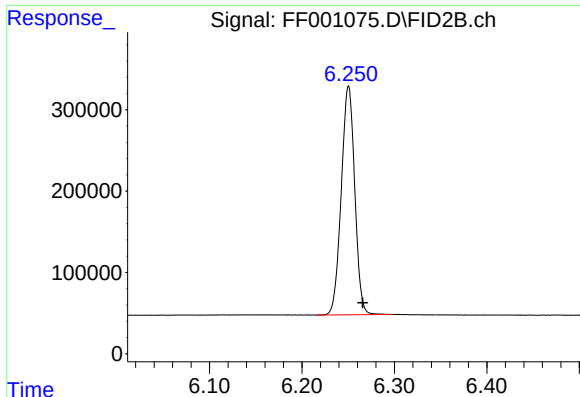

#3 N-DODECANE


R.T.: 6.250 min  
Delta R.T.: -0.015 min  
Response: 2847954  
Conc: 20.32 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

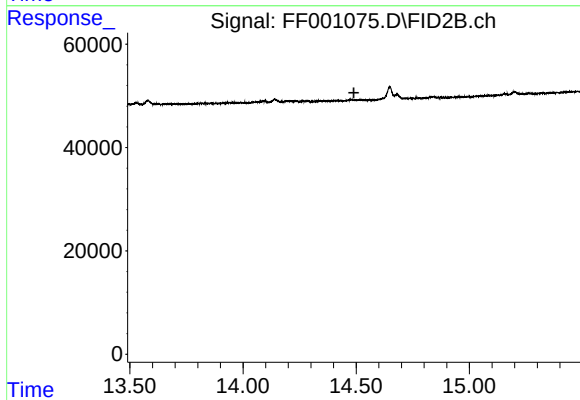

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.490 min  
Response: 0  
Conc: N.D.

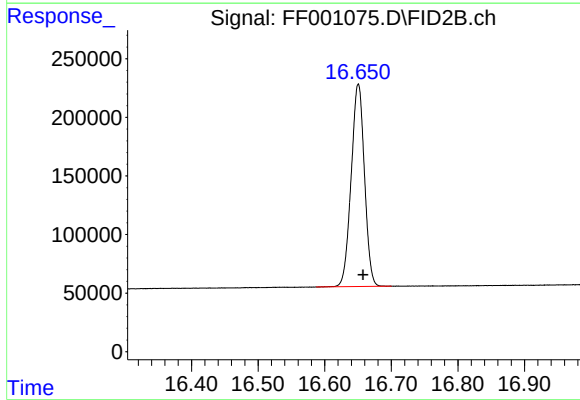

#12 N-OCTACOSANE

R.T.: 16.651 min  
Delta R.T.: -0.007 min  
Response: 2398198  
Conc: 18.86 ug/ml