

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
 Data File : FF001081.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2018 16:49
 Operator : UA\AJ
 Sample : J3631-03MSD
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 S83-0020MSD

Integration File: autoint1.e
 Quant Time: Jun 25 02:14:38 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.477	2165137	18.774 ug/ml
Target Compounds			
2) N-DECANE	4.240	2905244	20.734 ug/ml
3) N-DODECANE	6.252	3113355	22.214 ug/ml
4) N-TETRADECANE	8.041	2711031	19.472 ug/ml
5) N-HEXADECANE	9.637	2484012	18.016 ug/ml
6) N-OCTADECANE	11.076	2471554	18.099 ug/ml
7) N-EICOSANE	12.382	2418919	18.055 ug/ml
8) N-DOCOSANE	13.578	2367273	17.903 ug/ml
10) N-TETRACOSANE	14.680	2396652	18.477 ug/ml
11) N-HEXACOSANE	15.700	2350803	18.302 ug/ml
12) N-OCTACOSANE	16.649	2419658	19.029 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
Data File : FF001081.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2018 16:49
Operator : UA\AJ
Sample : J3631-03MSD
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
S83-0020MSD

Integration File: autoint1.e
Quant Time: Jun 25 02:14:38 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

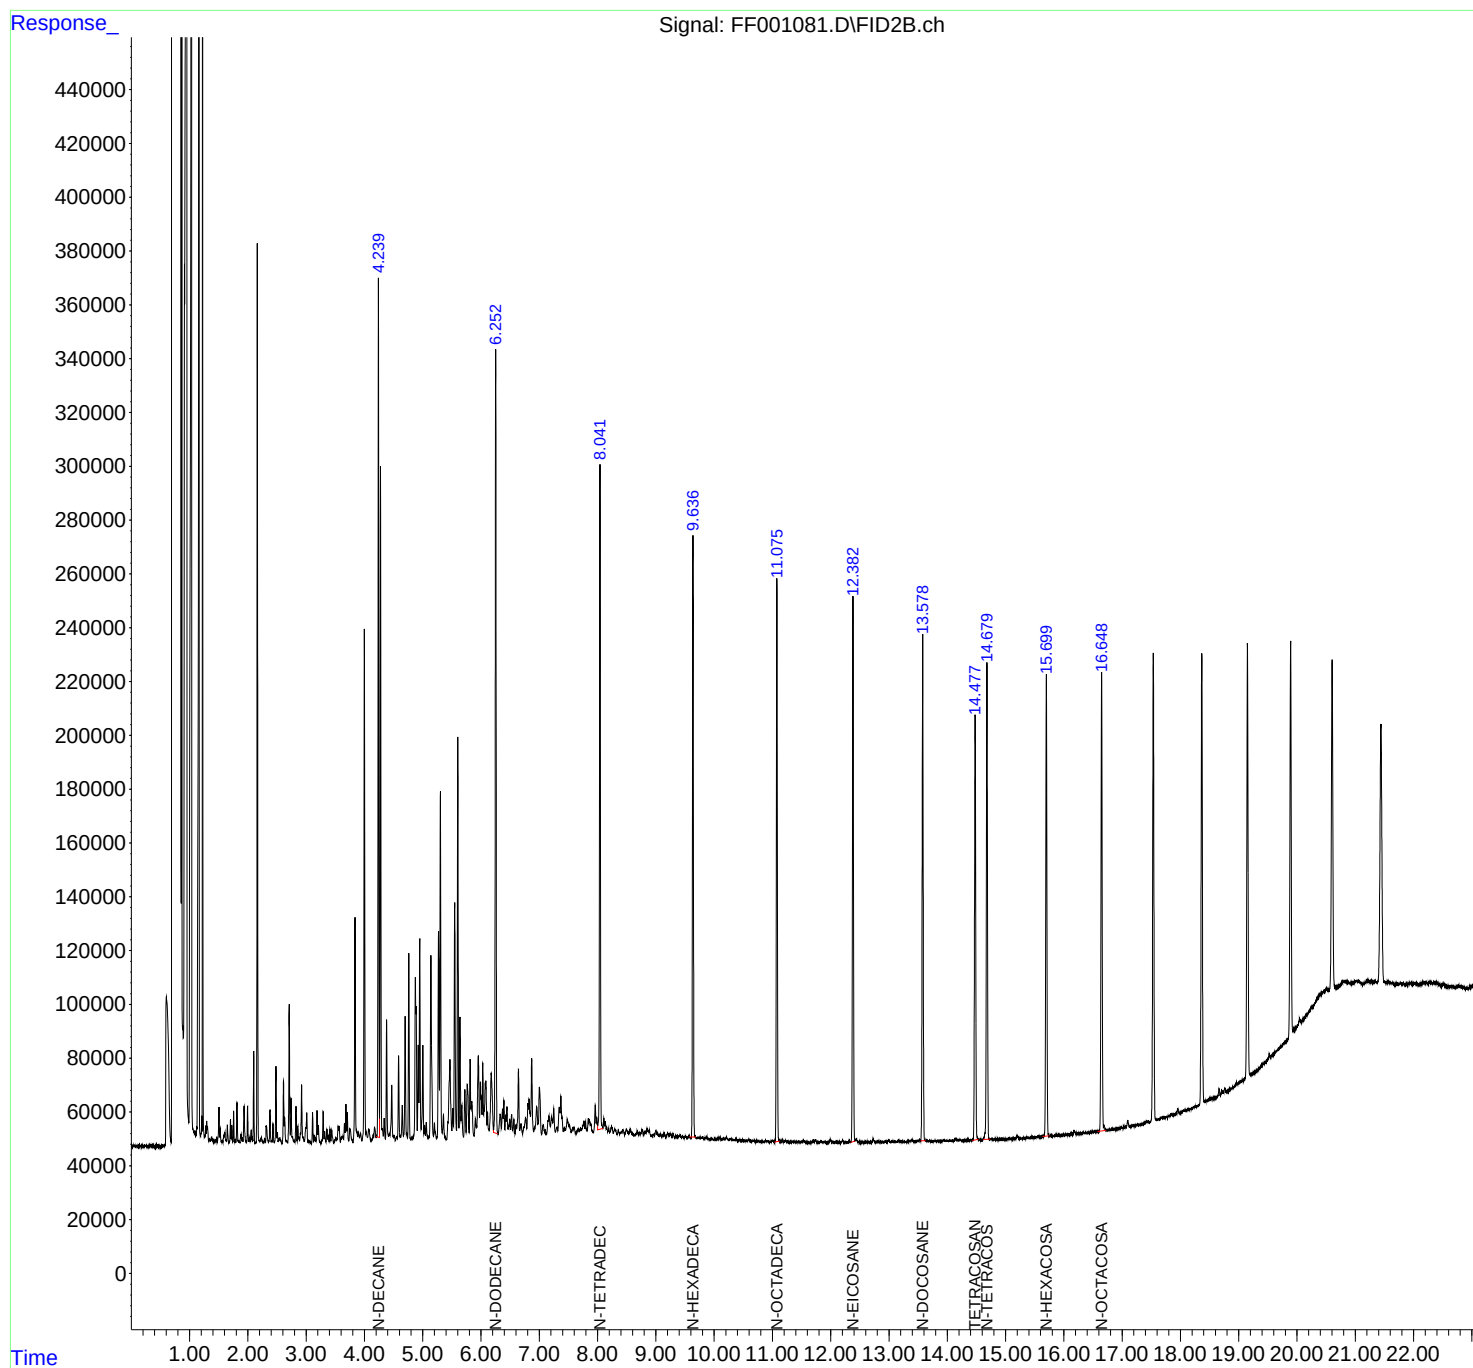


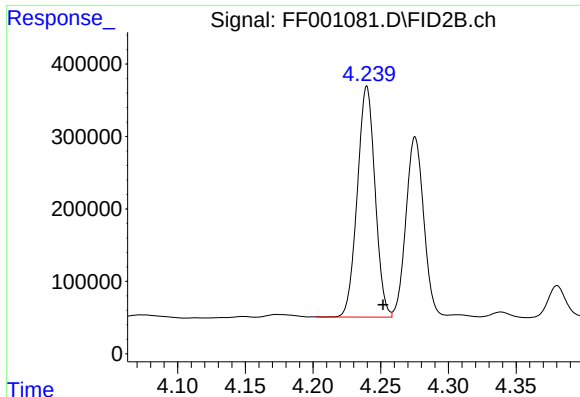

#2 N-DECANE


R.T.: 4.240 min
Delta R.T.: -0.012 min
Response: 2905244
Conc: 20.73 ug/ml

Instrument :
FID_F
ClientSampleId :
S83-0020MSD

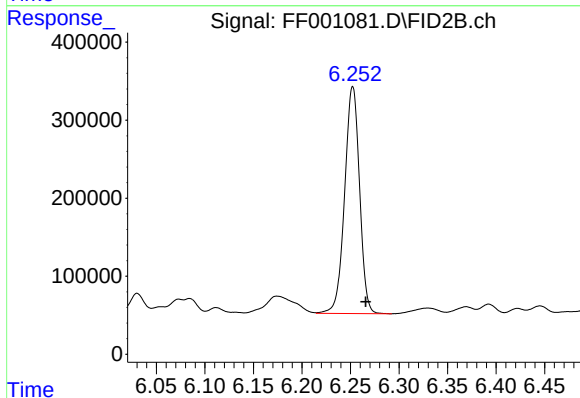


#3 N-DODECANE

R.T.: 6.252 min
Delta R.T.: -0.013 min
Response: 3113355
Conc: 22.21 ug/ml

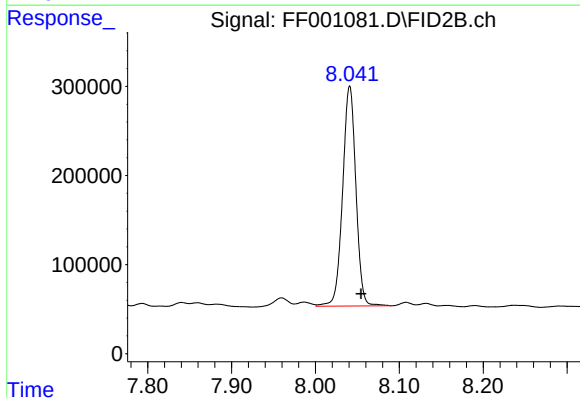


#4 N-TETRADECANE

R.T.: 8.041 min
Delta R.T.: -0.013 min
Response: 2711031
Conc: 19.47 ug/ml

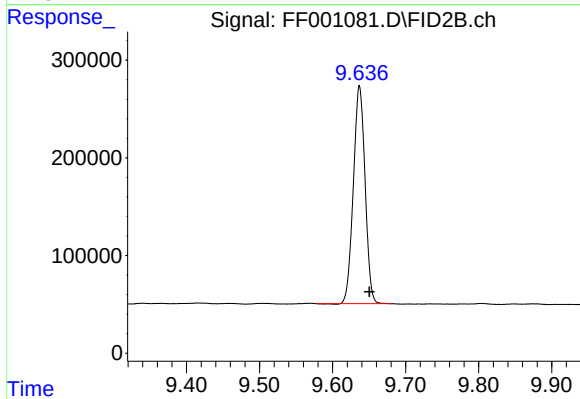

#5 N-HEXADECANE


R.T.: 9.637 min
Delta R.T.: -0.013 min
Response: 2484012
Conc: 18.02 ug/ml

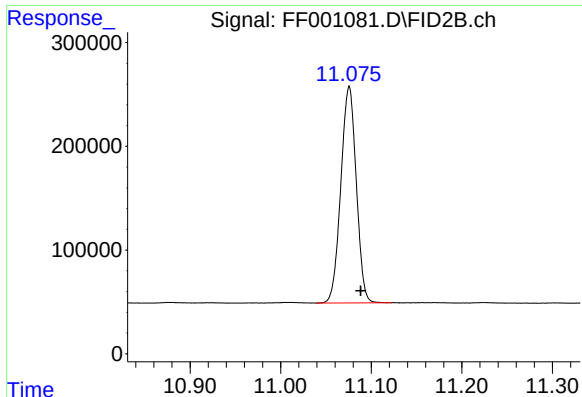

#6 N-OCTADECANE


R.T.: 11.076 min
Delta R.T.: -0.013 min
Response: 2471554
Conc: 18.10 ug/ml

Instrument :
FID_F
ClientSampleId :
S83-0020MSD

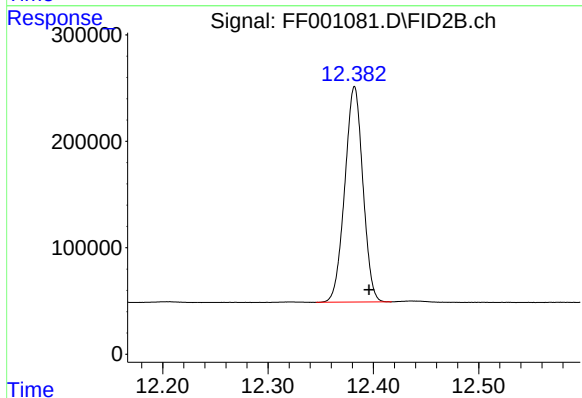


#7 N-EICOSANE

R.T.: 12.382 min
Delta R.T.: -0.014 min
Response: 2418919
Conc: 18.05 ug/ml

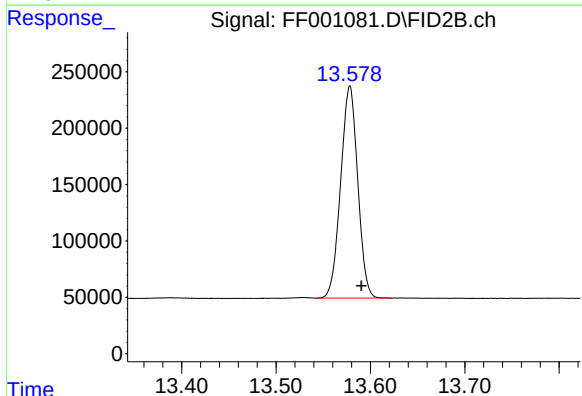


#8 N-DOCOSANE

R.T.: 13.578 min
Delta R.T.: -0.012 min
Response: 2367273
Conc: 17.90 ug/ml

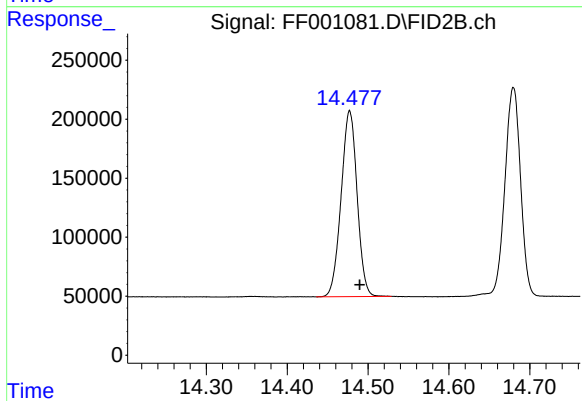

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.477 min
Delta R.T.: -0.012 min
Response: 2165137
Conc: 18.77 ug/ml

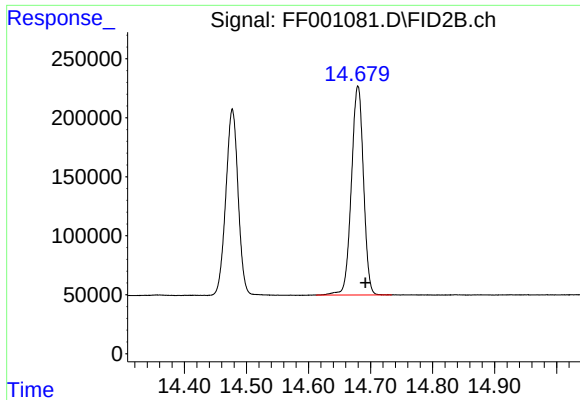

#10 N-TETRACOSANE


R.T.: 14.680 min
Delta R.T.: -0.012 min
Response: 2396652
Conc: 18.48 ug/ml

Instrument :
FID_F
ClientSampleId :
S83-0020MSD

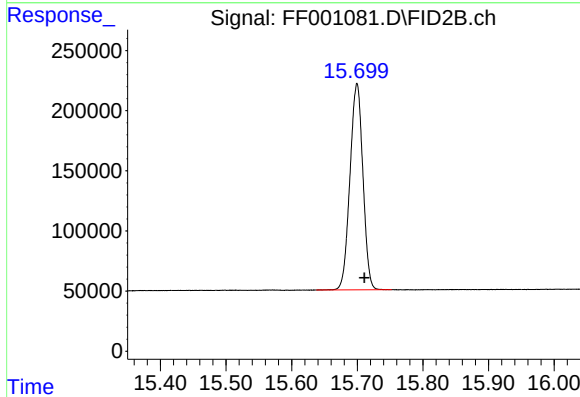

#11 N-HEXACOSANE

R.T.: 15.700 min
Delta R.T.: -0.011 min
Response: 2350803
Conc: 18.30 ug/ml

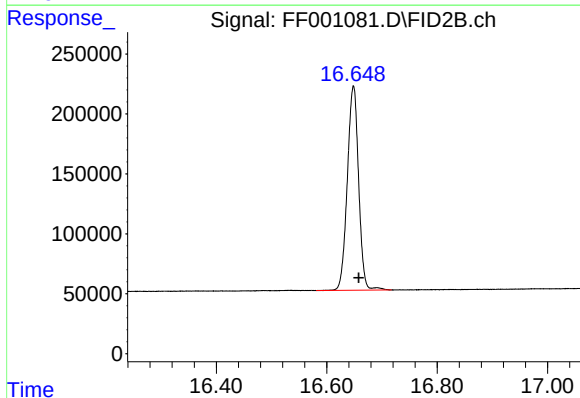

#12 N-OCTACOSANE

R.T.: 16.649 min
Delta R.T.: -0.009 min
Response: 2419658
Conc: 19.03 ug/ml