

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
Data File : FF001092.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2018 22:16
Operator : UA\AJ
Sample : J3688-02
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EPE-109-6(65-67)

Integration File: autoint1.e
Quant Time: Jun 25 04:04:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.472	1711443	14.840 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
Data File : FF001092.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2018 22:16
Operator : UA\AJ
Sample : J3688-02
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EPE-109-6(65-67)

Integration File: autoint1.e
Quant Time: Jun 25 04:04:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

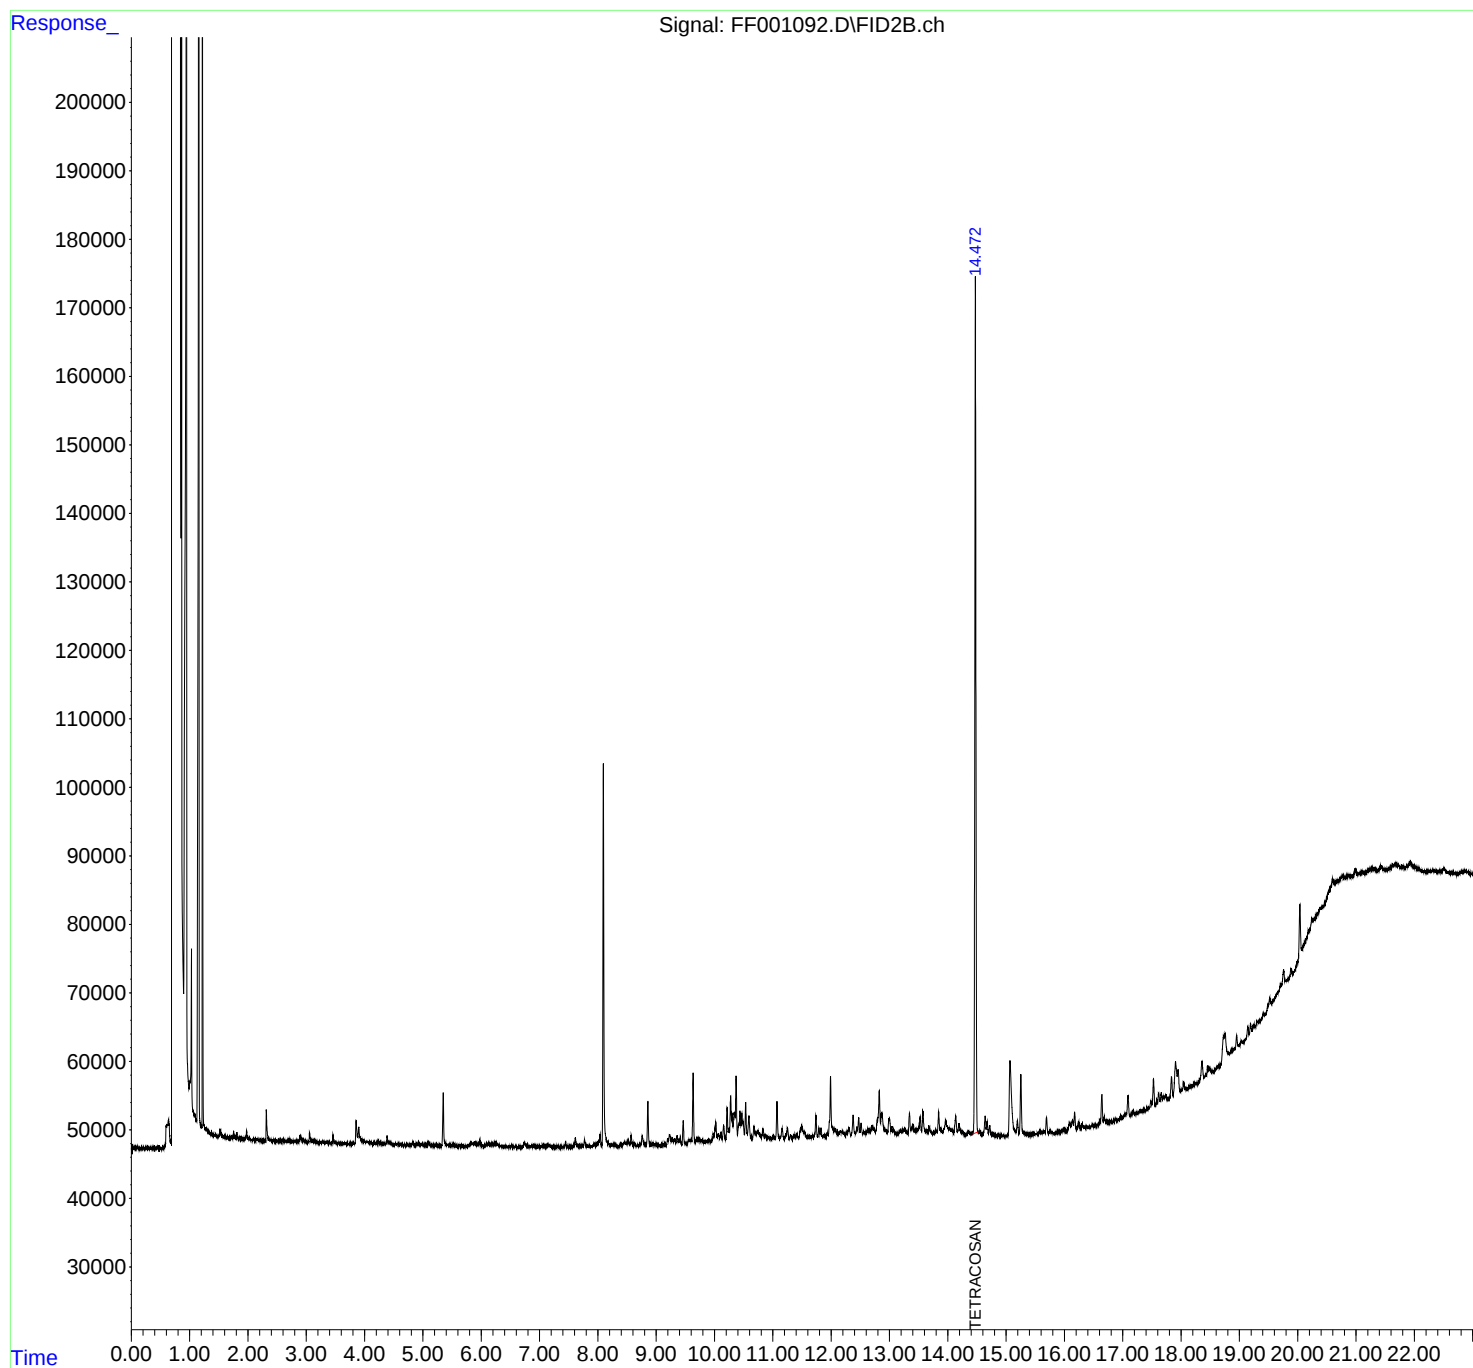

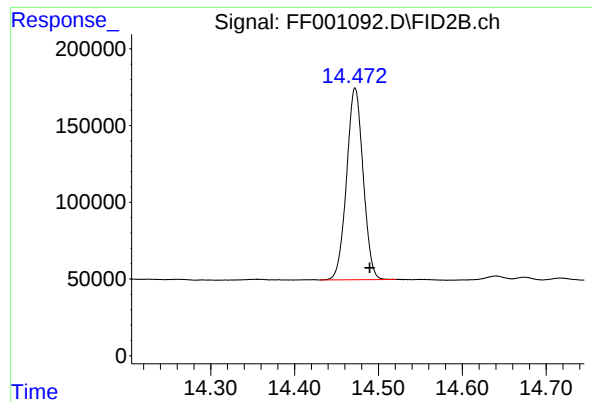

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.472 min
Delta R.T.: -0.018 min
Response: 1711443
Conc: 14.84 ug/ml

Instrument :
FID_F
ClientSampleId :
EPE-109-6(65-67)