

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
 Data File : FF001095.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2018 23:45
 Operator : UA\AJ
 Sample : PB110542BS
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB110542BS

Integration File: autoint1.e
 Quant Time: Jun 25 04:05:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.473	1825400	15.828 ug/ml
Target Compounds			
2) N-DECANE	4.238	3049525	21.764 ug/ml
3) N-DODECANE	6.250	2853978	20.363 ug/ml
4) N-TETRADECANE	8.038	2694736	19.355 ug/ml
5) N-HEXADECANE	9.634	2536983	18.400 ug/ml
6) N-OCTADECANE	11.072	2430596	17.800 ug/ml
7) N-EICOSANE	12.378	2335931	17.435 ug/ml
8) N-DOCOSANE	13.574	2282169	17.259 ug/ml
10) N-TETRACOSANE	14.675	2302067	17.748 ug/ml
11) N-HEXACOSANE	15.694	2262550	17.615 ug/ml
12) N-OCTACOSANE	16.643	2310224	18.168 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
Data File : FF001095.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2018 23:45
Operator : UA\AJ
Sample : PB110542BS
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB110542BS

Integration File: autoint1.e
Quant Time: Jun 25 04:05:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

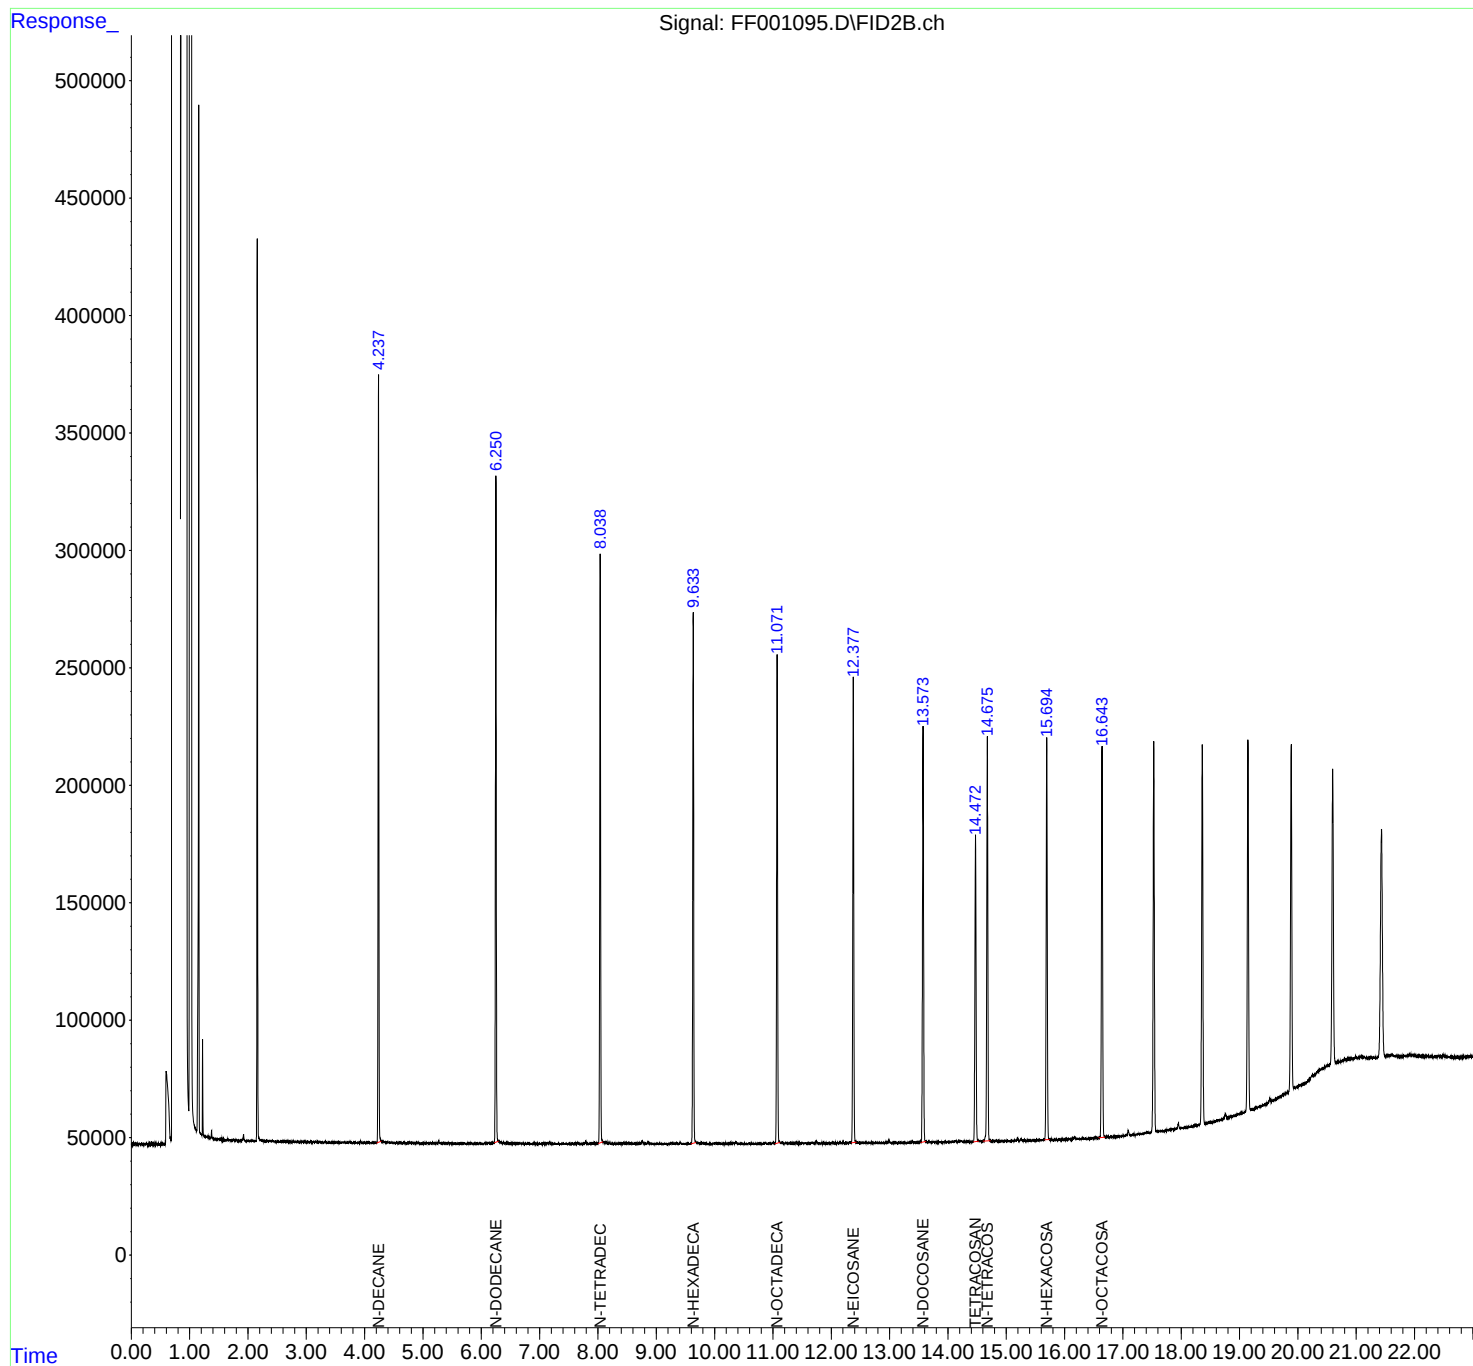


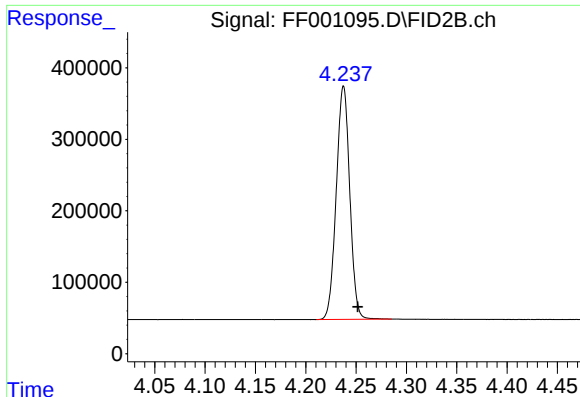

#2 N-DECANE


R.T.: 4.238 min
Delta R.T.: -0.014 min
Response: 3049525
Conc: 21.76 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110542BS

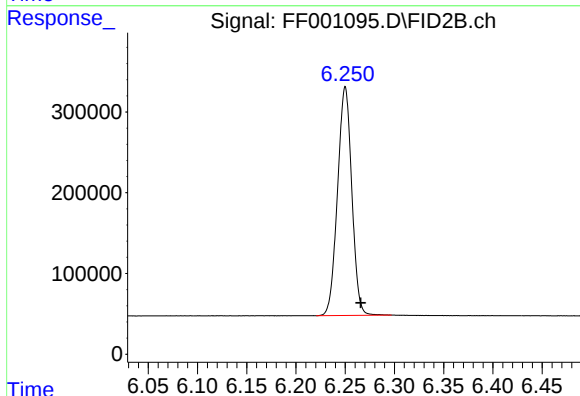


#3 N-DODECANE

R.T.: 6.250 min
Delta R.T.: -0.016 min
Response: 2853978
Conc: 20.36 ug/ml

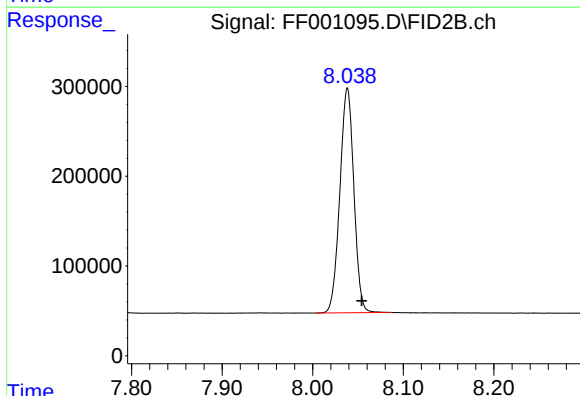


#4 N-TETRADECANE

R.T.: 8.038 min
Delta R.T.: -0.016 min
Response: 2694736
Conc: 19.35 ug/ml

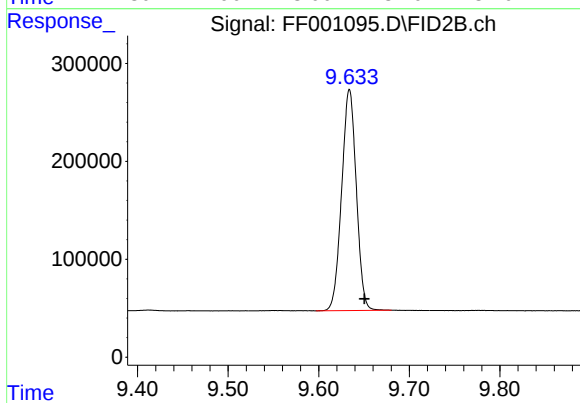

#5 N-HEXADECANE


R.T.: 9.634 min
Delta R.T.: -0.016 min
Response: 2536983
Conc: 18.40 ug/ml

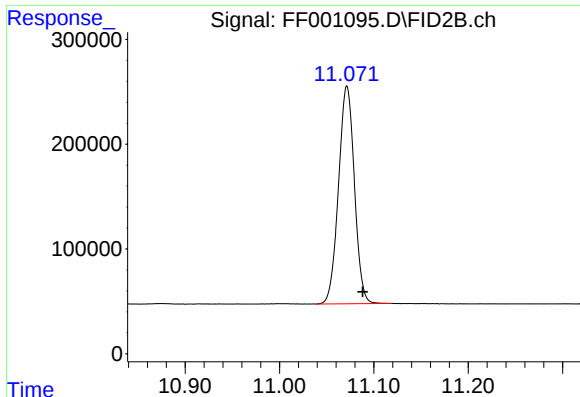

#6 N-OCTADECANE


R.T.: 11.072 min
Delta R.T.: -0.017 min
Response: 2430596
Conc: 17.80 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110542BS

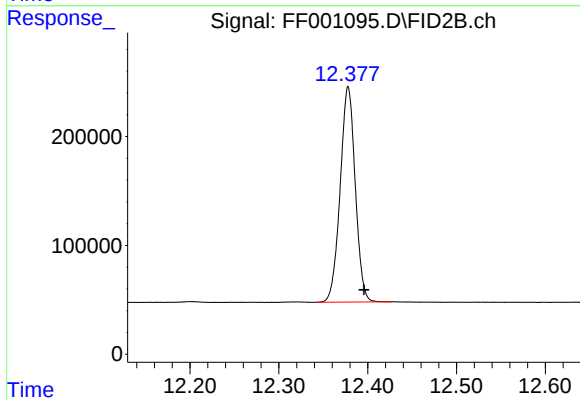


#7 N-EICOSANE

R.T.: 12.378 min
Delta R.T.: -0.018 min
Response: 2335931
Conc: 17.44 ug/ml

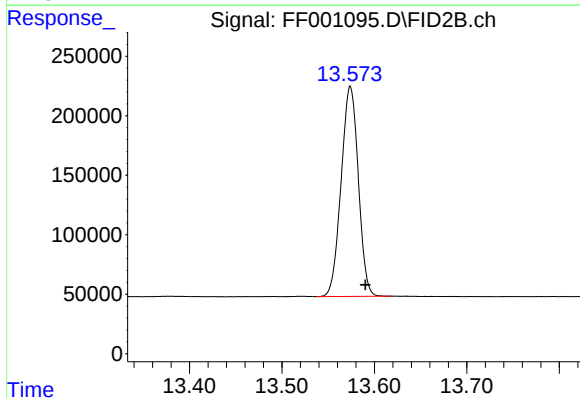


#8 N-DOCOSANE

R.T.: 13.574 min
Delta R.T.: -0.017 min
Response: 2282169
Conc: 17.26 ug/ml

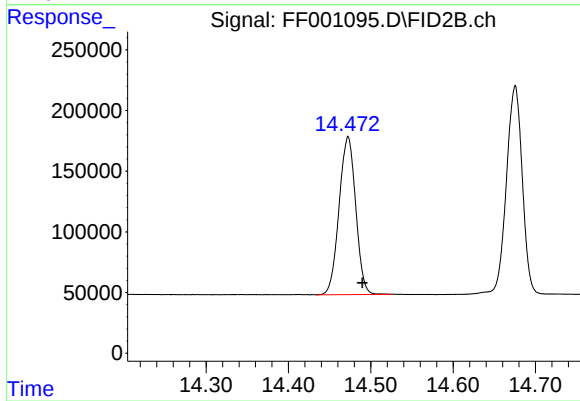

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.473 min
Delta R.T.: -0.017 min
Response: 1825400
Conc: 15.83 ug/ml

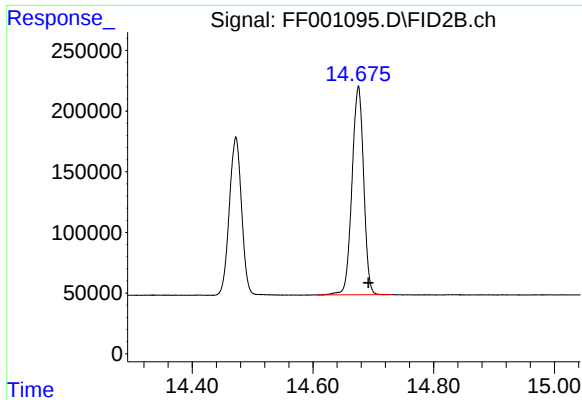

#10 N-TETRACOSANE


R.T.: 14.675 min
Delta R.T.: -0.016 min
Response: 2302067
Conc: 17.75 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110542BS

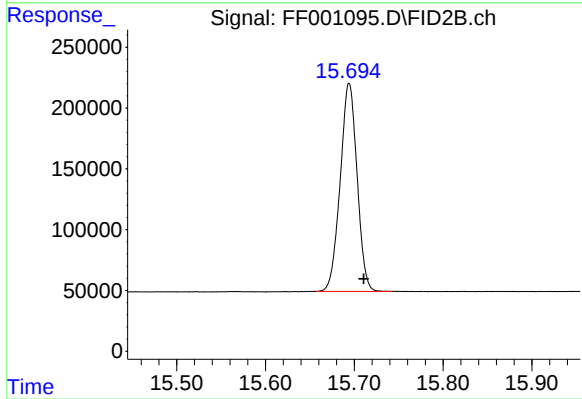

#11 N-HEXACOSANE

R.T.: 15.694 min
Delta R.T.: -0.016 min
Response: 2262550
Conc: 17.61 ug/ml

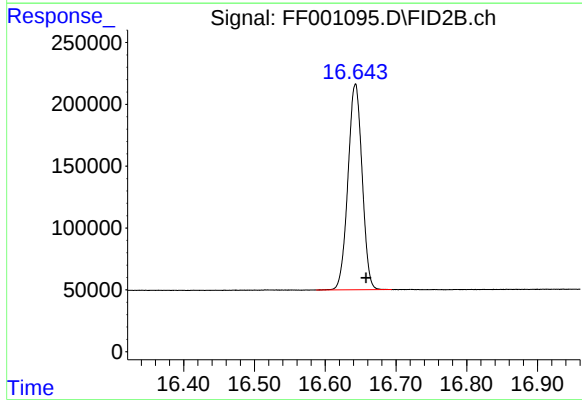

#12 N-OCTACOSANE

R.T.: 16.643 min
Delta R.T.: -0.015 min
Response: 2310224
Conc: 18.17 ug/ml