

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
 Data File : FF001097.D
 Signal(s) : FID2B.ch
 Acq On : 24 Jun 2018 00:45
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 04:05:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.474	5223137	45.291 ug/ml
Target Compounds			
2) N-DECANE	4.238	8201450	58.533 ug/ml
3) N-DODECANE	6.252	7597528	54.209 ug/ml
4) N-TETRADECANE	8.040	7089578	50.920 ug/ml
5) N-HEXADECANE	9.636	6687608	48.504 ug/ml
6) N-OCTADECANE	11.074	6389647	46.792 ug/ml
7) N-EICOSANE	12.380	6131611	45.766 ug/ml
8) N-DOCOSANE	13.576	5992776	45.322 ug/ml
10) N-TETRACOSANE	14.677	5965020	45.988 ug/ml
11) N-HEXACOSANE	15.697	5982147	46.574 ug/ml
12) N-OCTACOSANE	16.645	6084267	47.848 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062318\
Data File : FF001097.D
Signal(s) : FID2B.ch
Acq On : 24 Jun 2018 00:45
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:05:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

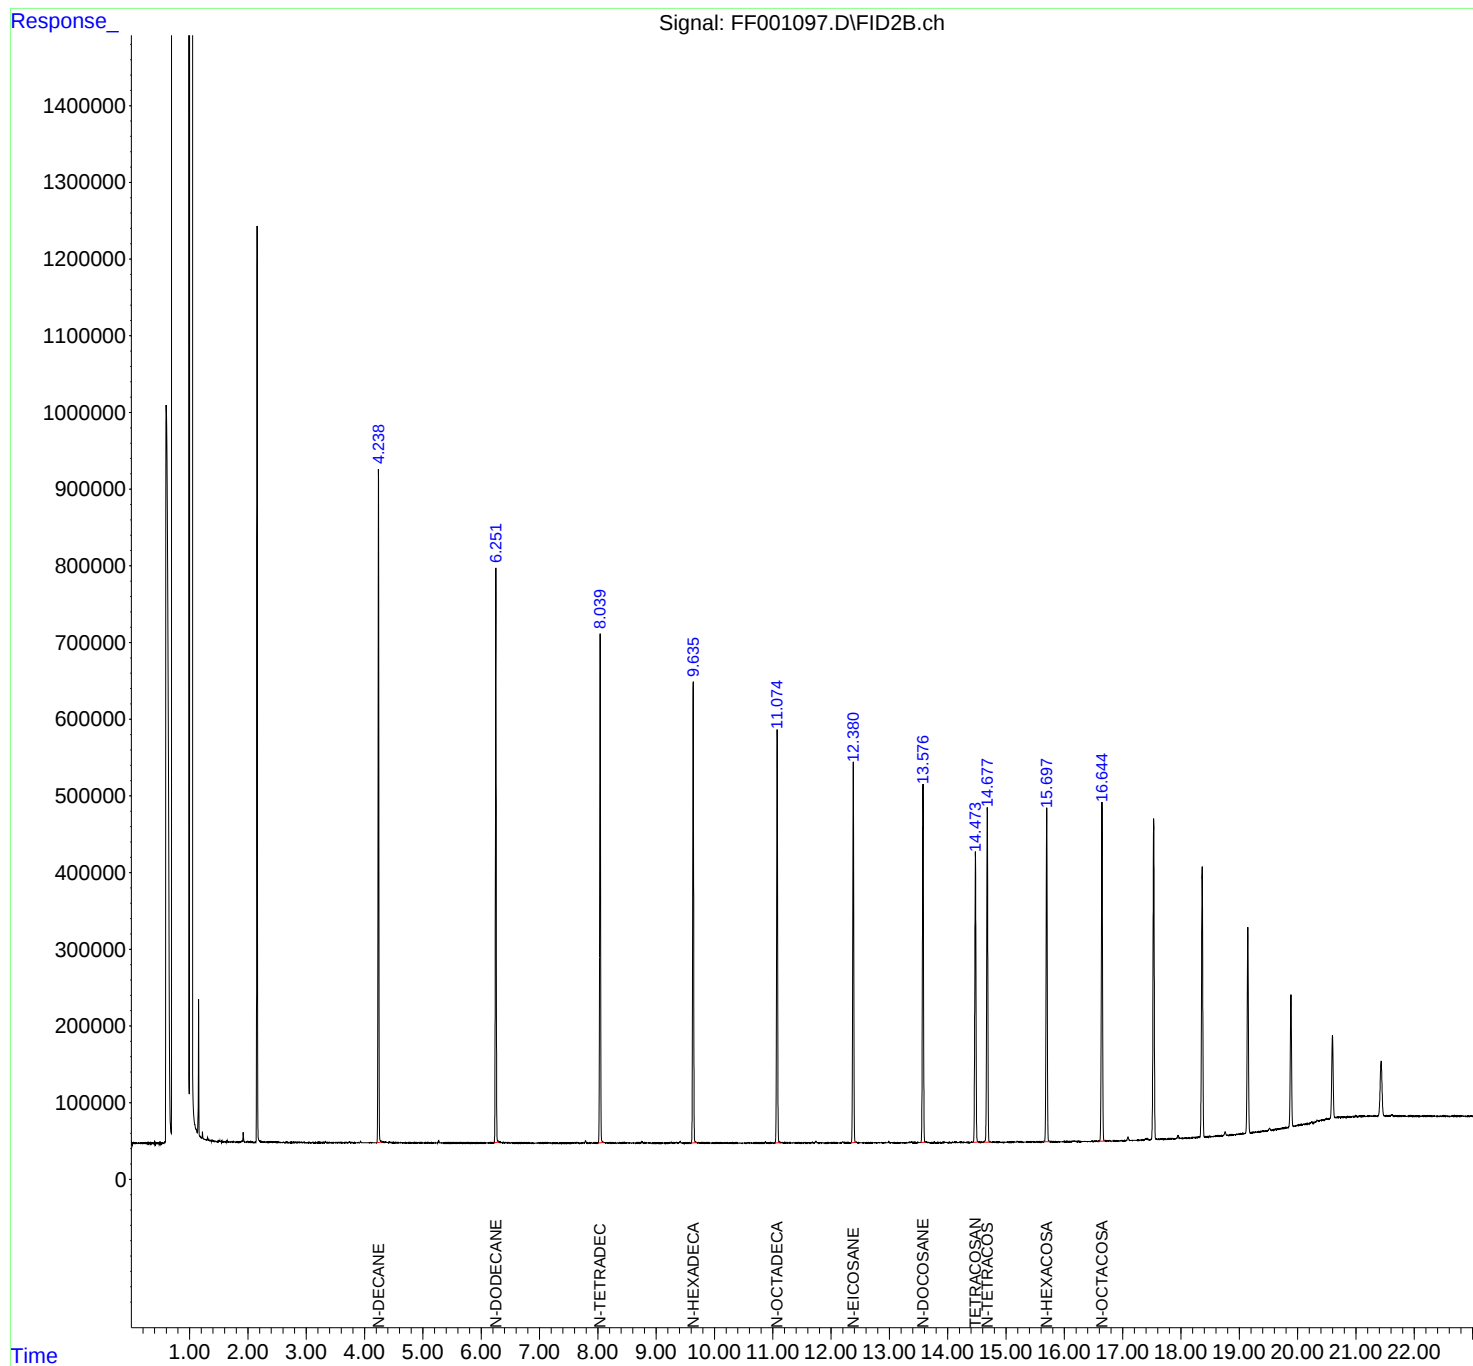


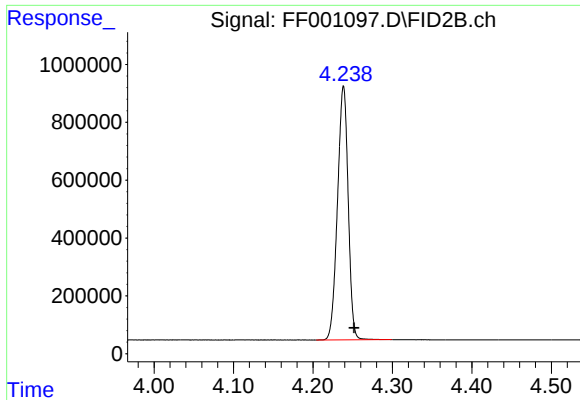

#2 N-DECANE


R.T.: 4.238 min
Delta R.T.: -0.013 min
Response: 8201450
Conc: 58.53 ug/ml

Instrument :
FID_F
ClientSampleId :

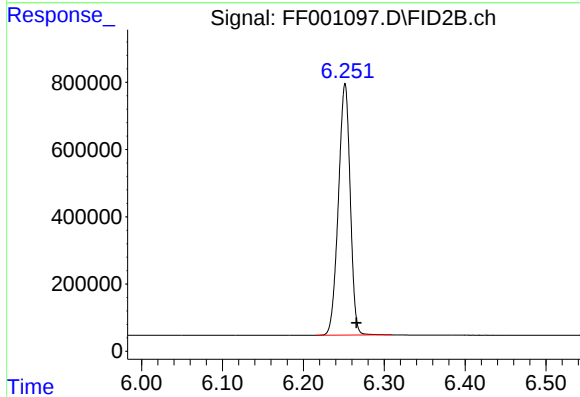


#3 N-DODECANE

R.T.: 6.252 min
Delta R.T.: -0.014 min
Response: 7597528
Conc: 54.21 ug/ml

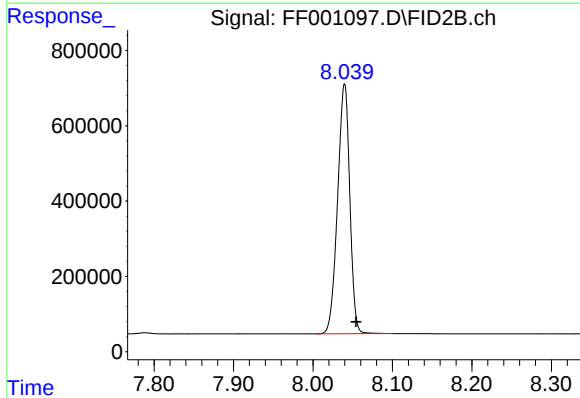


#4 N-TETRADECANE

R.T.: 8.040 min
Delta R.T.: -0.014 min
Response: 7089578
Conc: 50.92 ug/ml

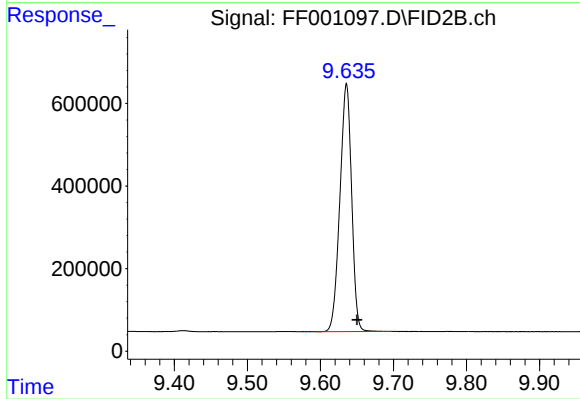

#5 N-HEXADECANE


R.T.: 9.636 min
Delta R.T.: -0.014 min
Response: 6687608
Conc: 48.50 ug/ml

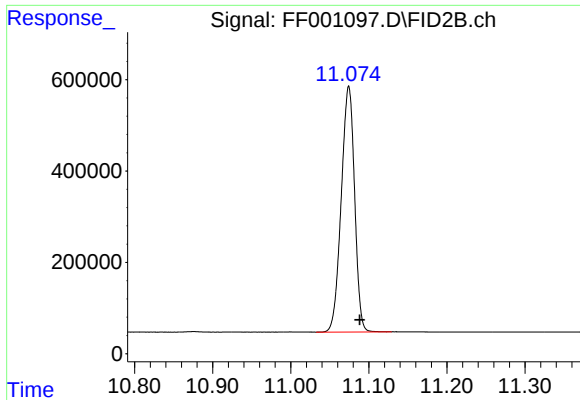

#6 N-OCTADECANE


R.T.: 11.074 min
Delta R.T.: -0.014 min
Response: 6389647
Conc: 46.79 ug/ml

Instrument :
FID_F
ClientSampleId :

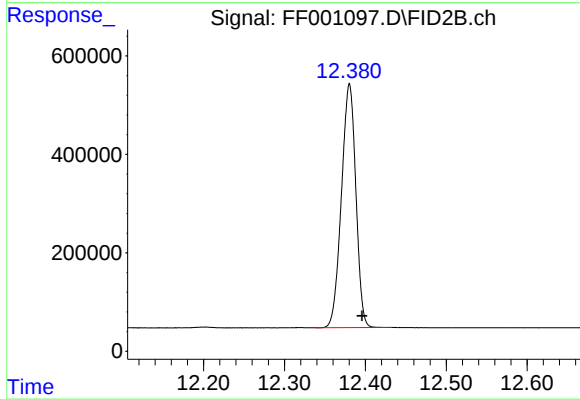


#7 N-EICOSANE

R.T.: 12.380 min
Delta R.T.: -0.016 min
Response: 6131611
Conc: 45.77 ug/ml

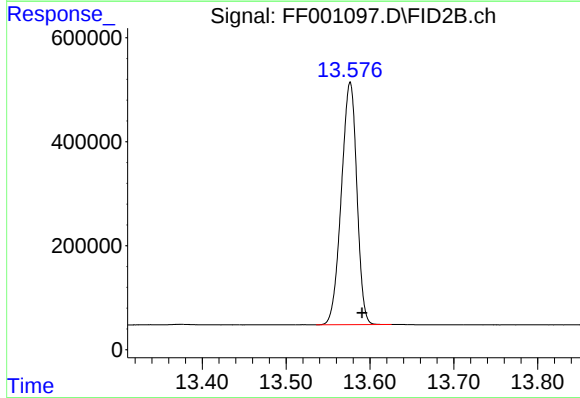


#8 N-DOCOSANE

R.T.: 13.576 min
Delta R.T.: -0.014 min
Response: 5992776
Conc: 45.32 ug/ml

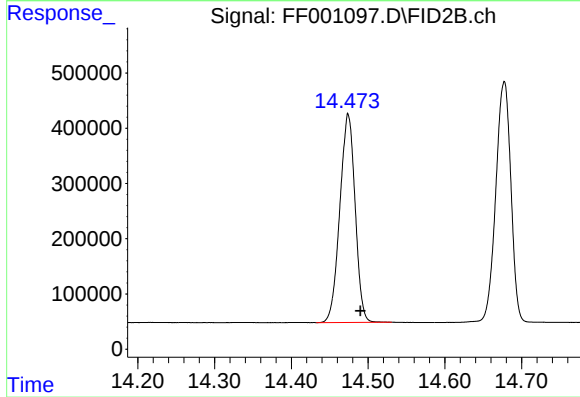

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.474 min
Delta R.T.: -0.016 min
Response: 5223137
Conc: 45.29 ug/ml

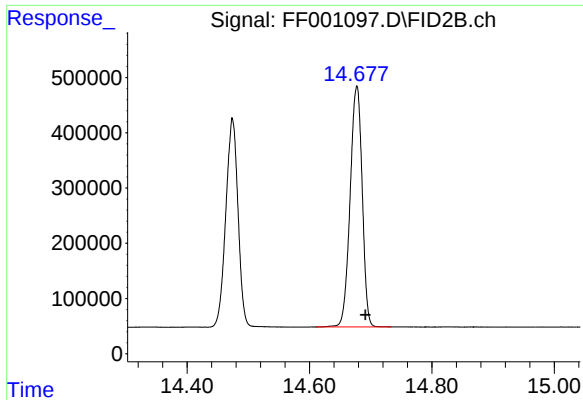

#10 N-TETRACOSANE


R.T.: 14.677 min
Delta R.T.: -0.014 min
Response: 5965020
Conc: 45.99 ug/ml

Instrument :
FID_F
ClientSampleId :

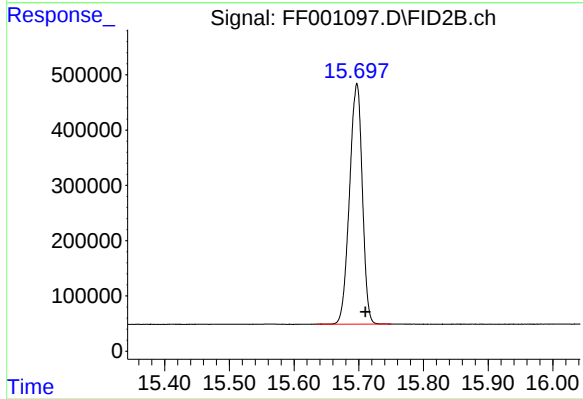

#11 N-HEXACOSANE

R.T.: 15.697 min
Delta R.T.: -0.013 min
Response: 5982147
Conc: 46.57 ug/ml

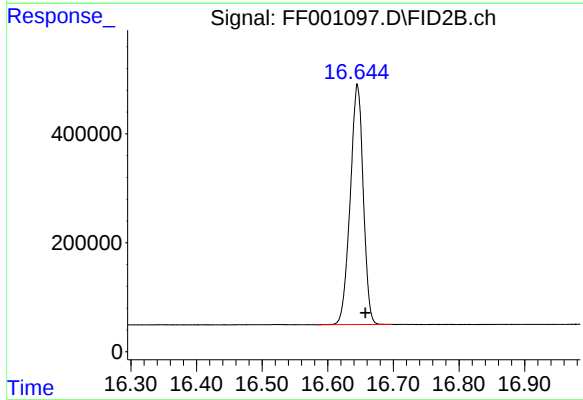

#12 N-OCTACOSANE

R.T.: 16.645 min
Delta R.T.: -0.013 min
Response: 6084267
Conc: 47.85 ug/ml