

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062320\
 Data File : FF007105.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2020 10:26
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 00:59:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
 Quant Title :
 QLast Update : Tue Jun 16 04:06:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.487	3090246	22.520 ug/ml
12) N-OCTACOSANE	16.925	2998574	20.113 ug/ml
13) N-TRIACONTANE	17.814	237626	1.584 ug/ml
14) N-DOTRIACONTANE	18.648	252848	1.830 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062320\
Data File : FF007105.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2020 10:26
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 00:59:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

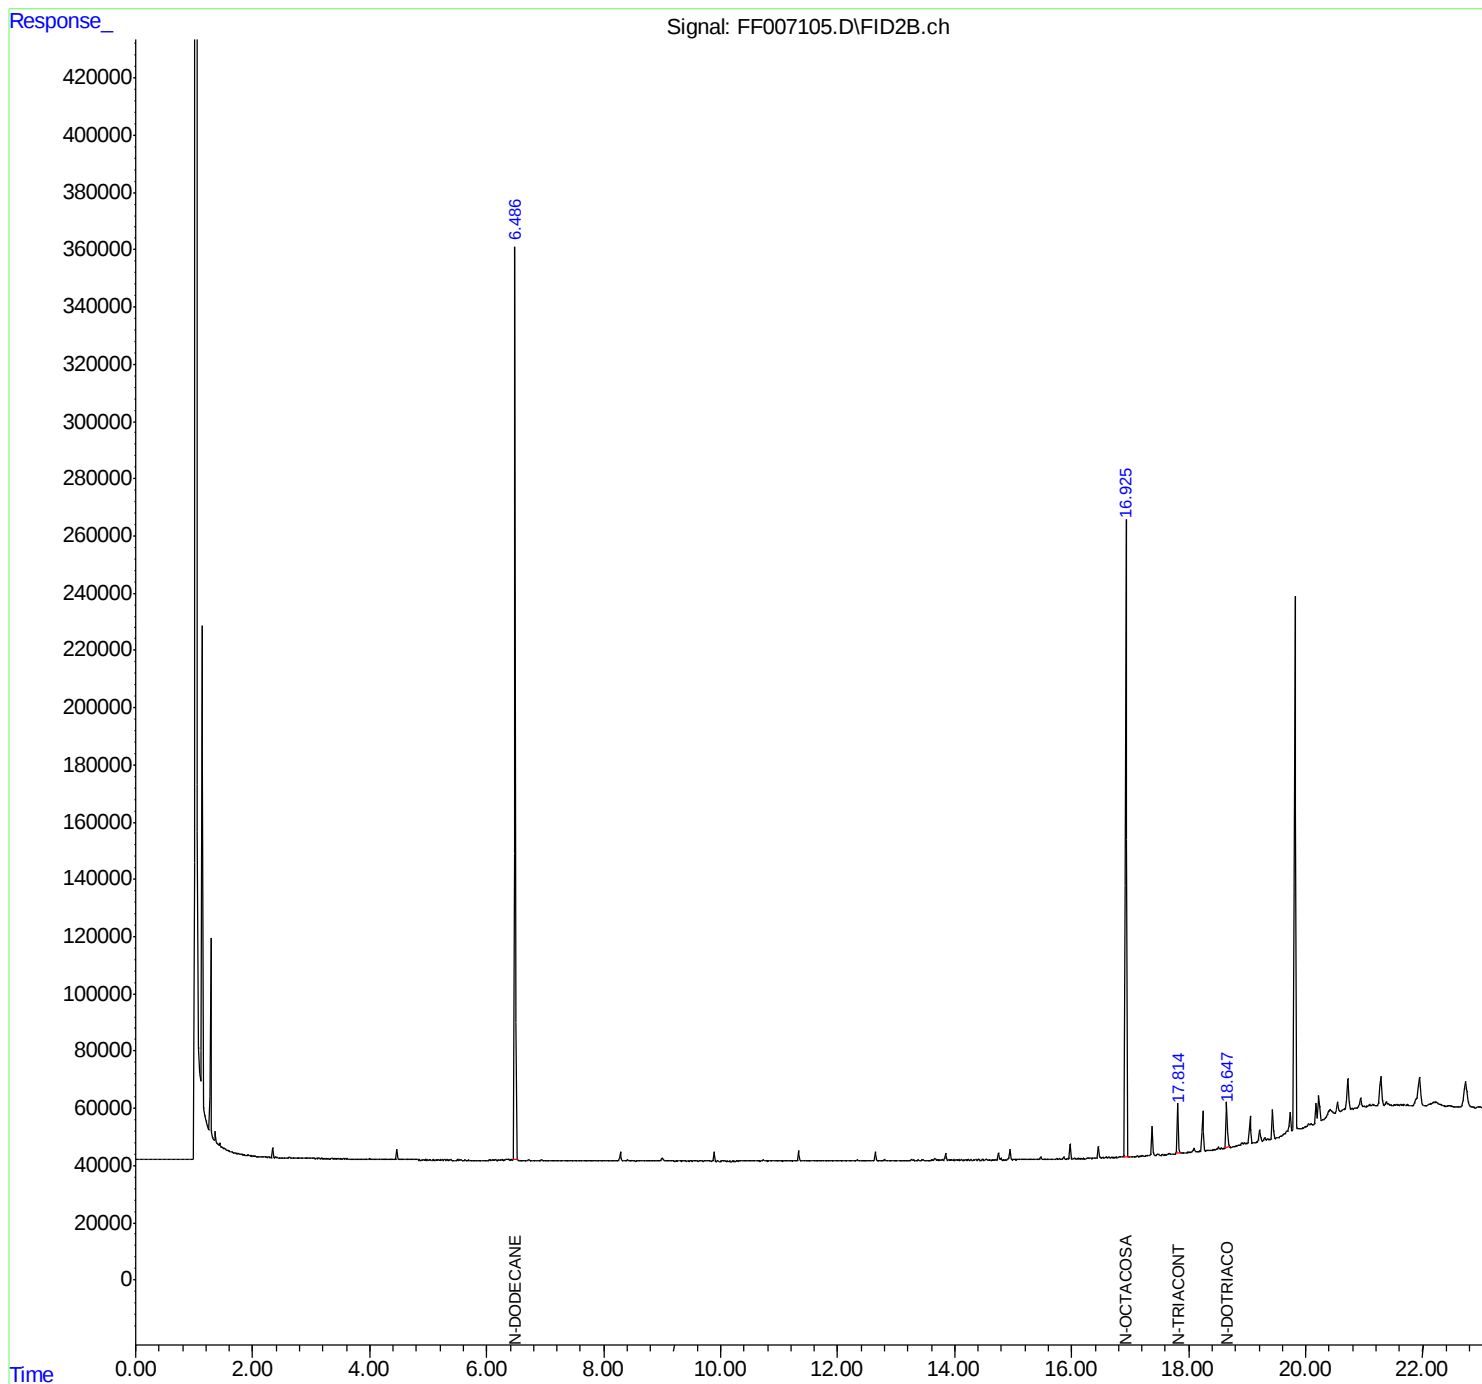


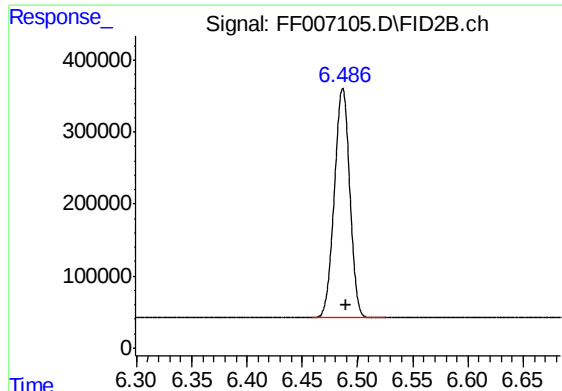

#3 N-DODECANE


R.T.: 6.487 min
Delta R.T.: -0.003 min
Response: 3090246
Conc: 22.52 ug/ml

Instrument :
FID_F
ClientSampleId :

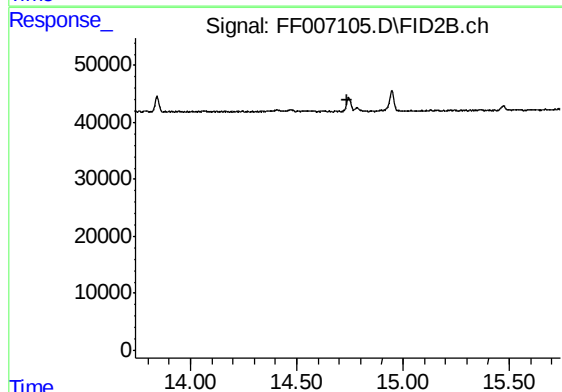


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.741 min
Response: 0
Conc: N.D.

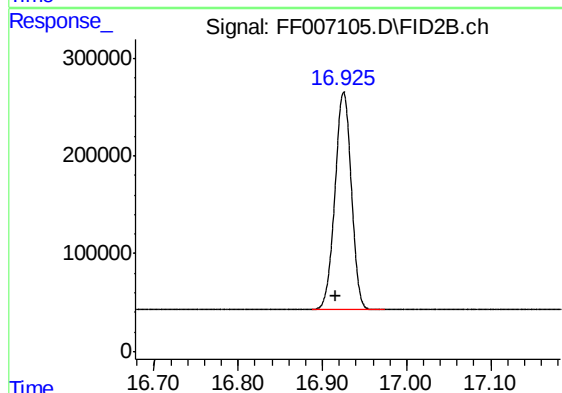


#12 N-OCTACOSANE

R.T.: 16.925 min
Delta R.T.: 0.009 min
Response: 2998574
Conc: 20.11 ug/ml

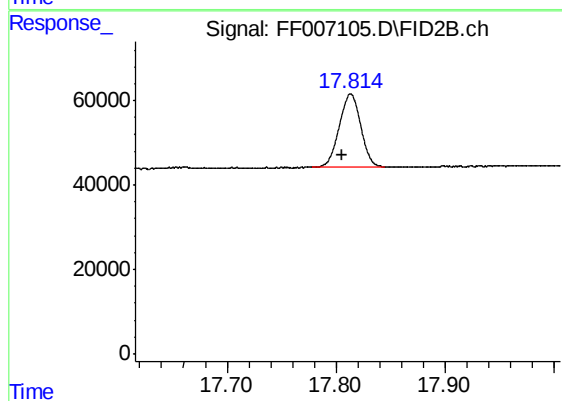

#13 N-TRIACONTANE

R.T.: 17.814 min
Delta R.T.: 0.008 min
Response: 237626
Conc: 1.58 ug/ml

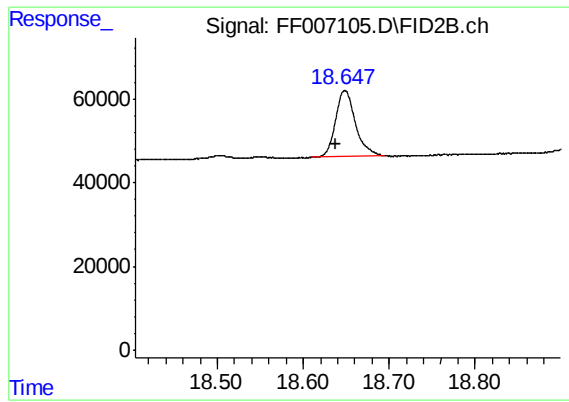

#14 N-DOTRIACONTANE

R.T.:	18.648 min
Delta R.T.:	0.009 min
Response:	252848
Conc:	1.83 ug/ml

Instrument :
FID_F
ClientSampleId :