

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062320\
 Data File : FF007108.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2020 11:59
 Operator : DD\AJ
 Sample : L3081-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 01:00:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
 Quant Title :
 QLast Update : Tue Jun 16 04:06:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	2270480	19.287 ug/ml
Target Compounds			
4) N-TETRADECANE	8.344f	265619	1.943 ug/ml
7) N-EICOSANE	12.643	229267	1.678 ug/ml
8) N-DOCOSANE	13.876	675930	4.960 ug/ml
10) N-TETRACOSANE	14.932	1500064	9.122 ug/ml
11) N-HEXACOSANE	15.990	1544563	10.793 ug/ml
12) N-OCTACOSANE	16.931	6141129	41.192 ug/ml
13) N-TRIACONTANE	17.823	10030426	66.842 ug/ml
14) N-DOTRIACONTANE	18.664	4644215	33.614 ug/ml
15) N-TETRATRIACONTANE	19.396	1932917	17.423 ug/ml
16) N-HEXATRIACONTANE	20.166	1065225	12.898 ug/ml
17) N-OCTATRIACONTANE	20.964	233469	3.416 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062320\
Data File : FF007108.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2020 11:59
Operator : DD\AJ
Sample : L3081-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:00:00 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

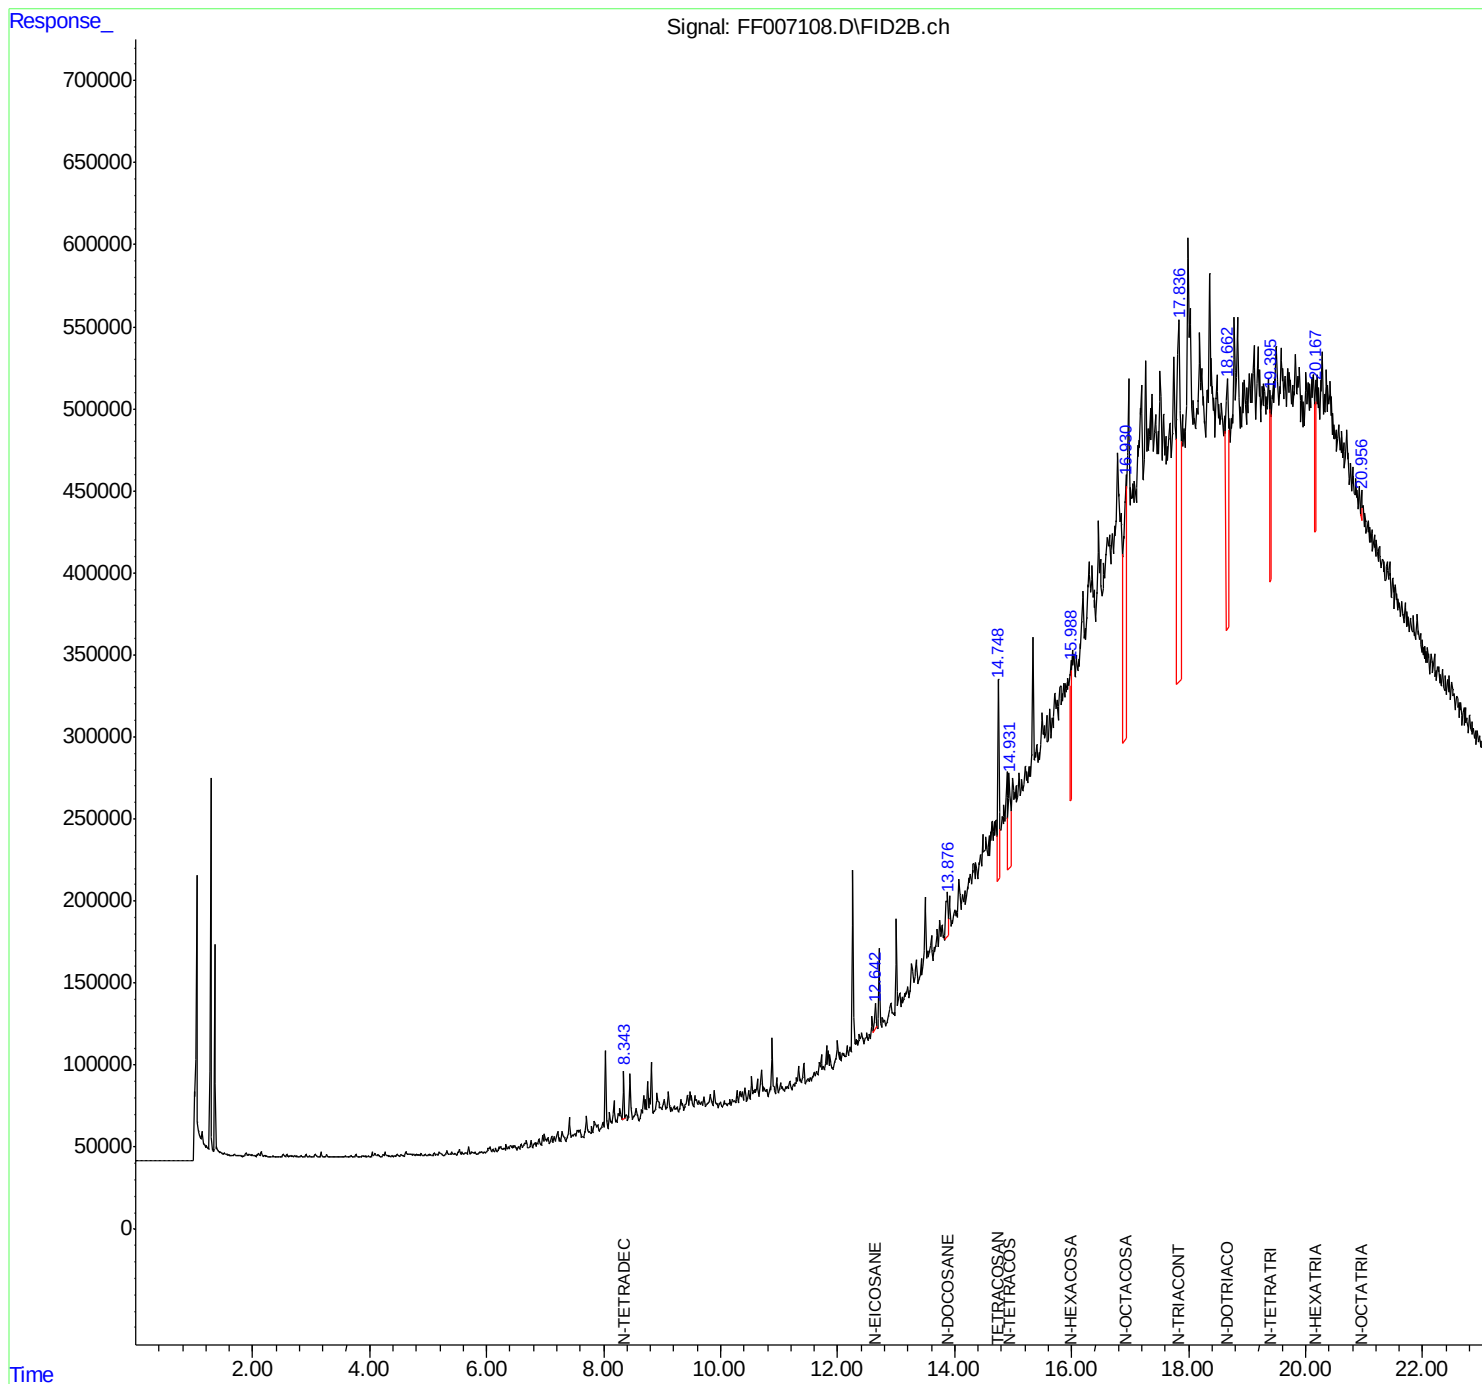


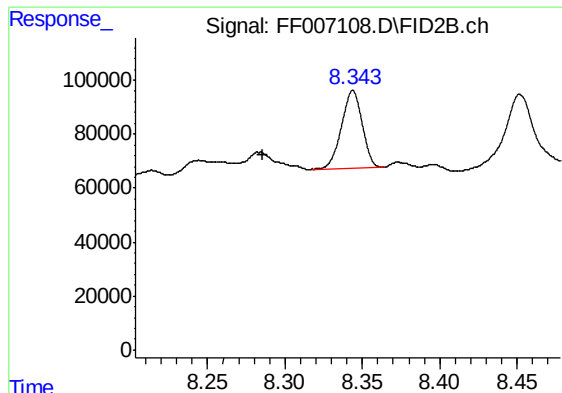

#4 N-TETRADECANE


R.T.: 8.344 min
Delta R.T.: 0.058 min
Response: 265619
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :

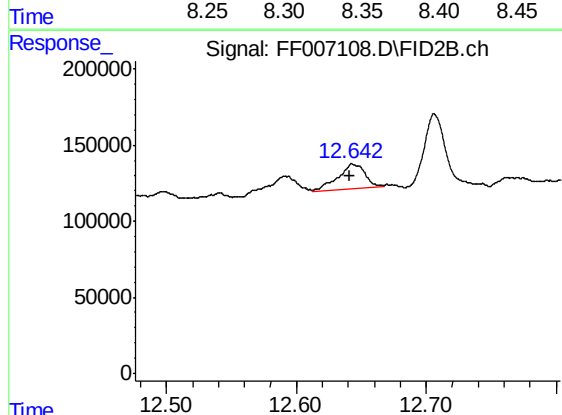


#7 N-EICOSANE

R.T.: 12.643 min
Delta R.T.: 0.002 min
Response: 229267
Conc: 1.68 ug/ml

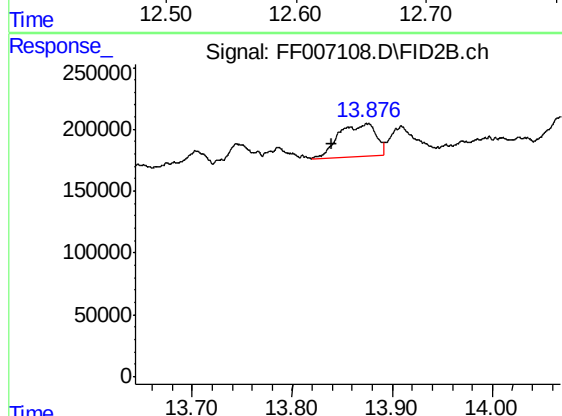


#8 N-DOCOSANE

R.T.: 13.876 min
Delta R.T.: 0.036 min
Response: 675930
Conc: 4.96 ug/ml

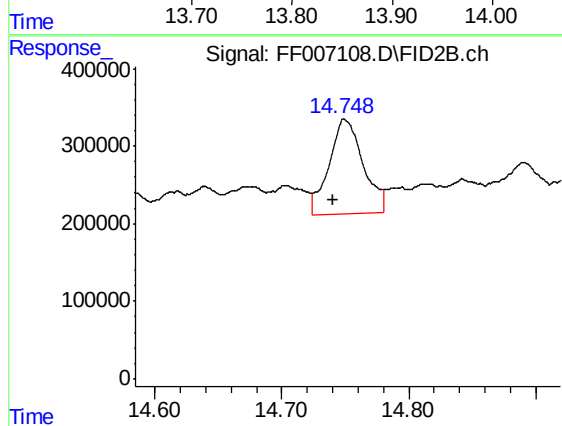

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.749 min
Delta R.T.: 0.009 min
Response: 2270480
Conc: 19.29 ug/ml

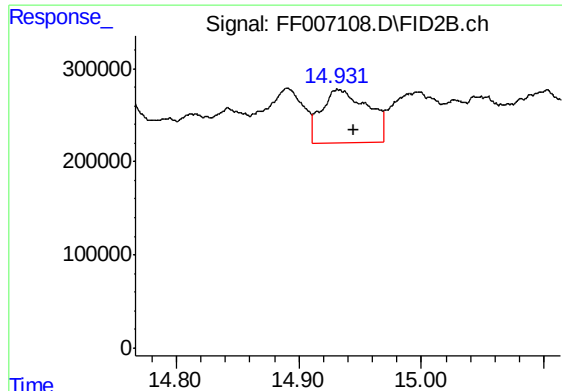

#10 N-TETRACOSANE


R.T.: 14.932 min
Delta R.T.: -0.013 min
Response: 1500064
Conc: 9.12 ug/ml

Instrument :
FID_F
ClientSampleId :

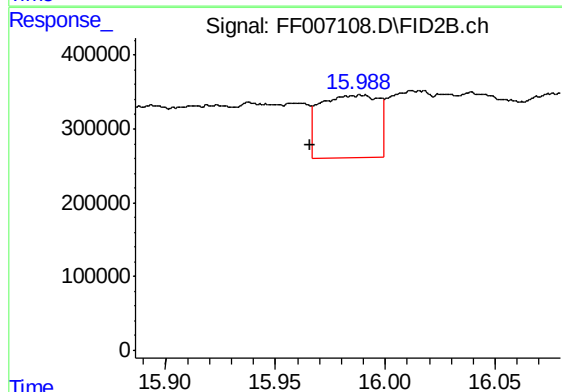


#11 N-HEXACOSANE

R.T.: 15.990 min
Delta R.T.: 0.024 min
Response: 1544563
Conc: 10.79 ug/ml

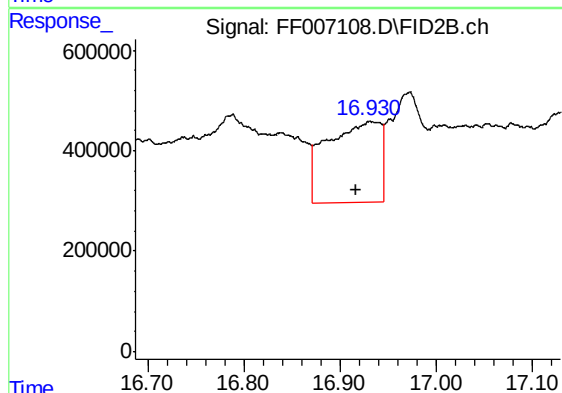


#12 N-OCTACOSANE

R.T.: 16.931 min
Delta R.T.: 0.015 min
Response: 6141129
Conc: 41.19 ug/ml

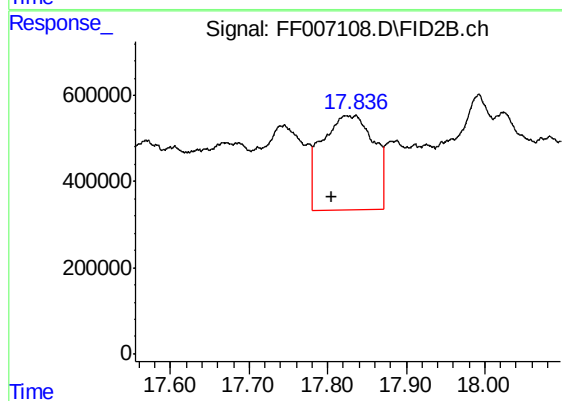

#13 N-TRIACONTANE


R.T.: 17.823 min
Delta R.T.: 0.018 min
Response: 10030426
Conc: 66.84 ug/ml

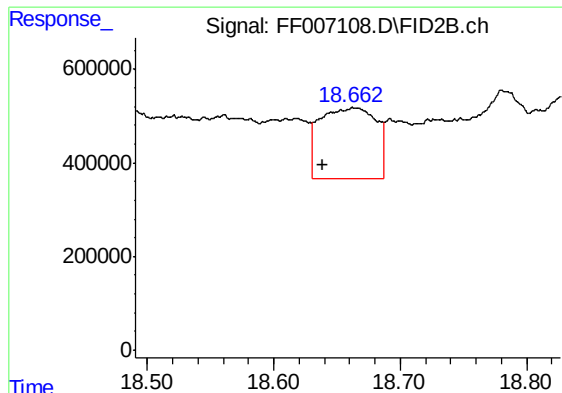

#14 N-DOTRIACONTANE


R.T.: 18.664 min
Delta R.T.: 0.026 min
Response: 4644215
Conc: 33.61 ug/ml

Instrument :
FID_F
ClientSampleId :

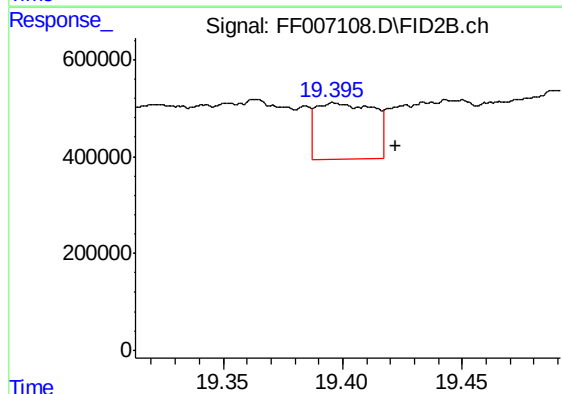


#15 N-TETRATRIACONTANE

R.T.: 19.396 min
Delta R.T.: -0.026 min
Response: 1932917
Conc: 17.42 ug/ml

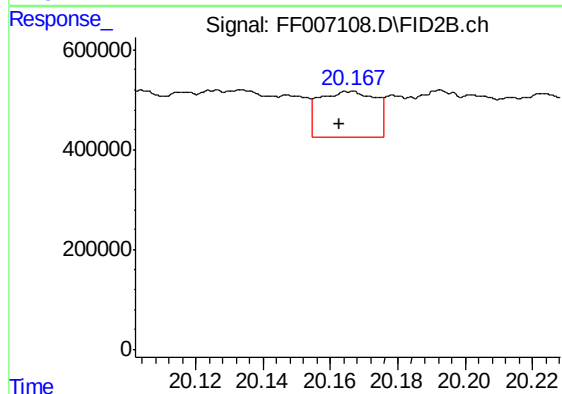

#16 N-HEXATRIACONTANE

R.T.: 20.166 min
Delta R.T.: 0.003 min
Response: 1065225
Conc: 12.90 ug/ml

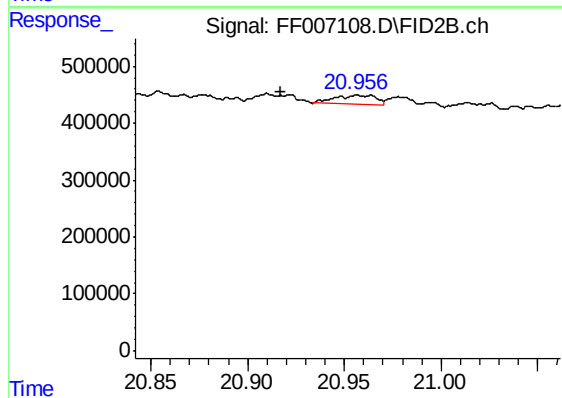

#17 N-OCTATRIACONTANE

R.T.: 20.964 min
Delta R.T.: 0.047 min
Response: 233469
Conc: 3.42 ug/ml