

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062320\
Data File : FF007109.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2020 12:30
Operator : DD\AJ
Sample : L3081-01 20X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 24 01:00:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	84600	0.719 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

Ankita
6/25/2020 8:05:34 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062320\
Data File : FF007109.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2020 12:30
Operator : DD\AJ
Sample : L3081-01 20X
Misc :
ALS Vial : 58 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :


Manual Integrations
APPROVED

Ankita
6/25/2020 8:05:34 AM

Integration File: autoint1.e
Quant Time: Jun 24 01:00:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

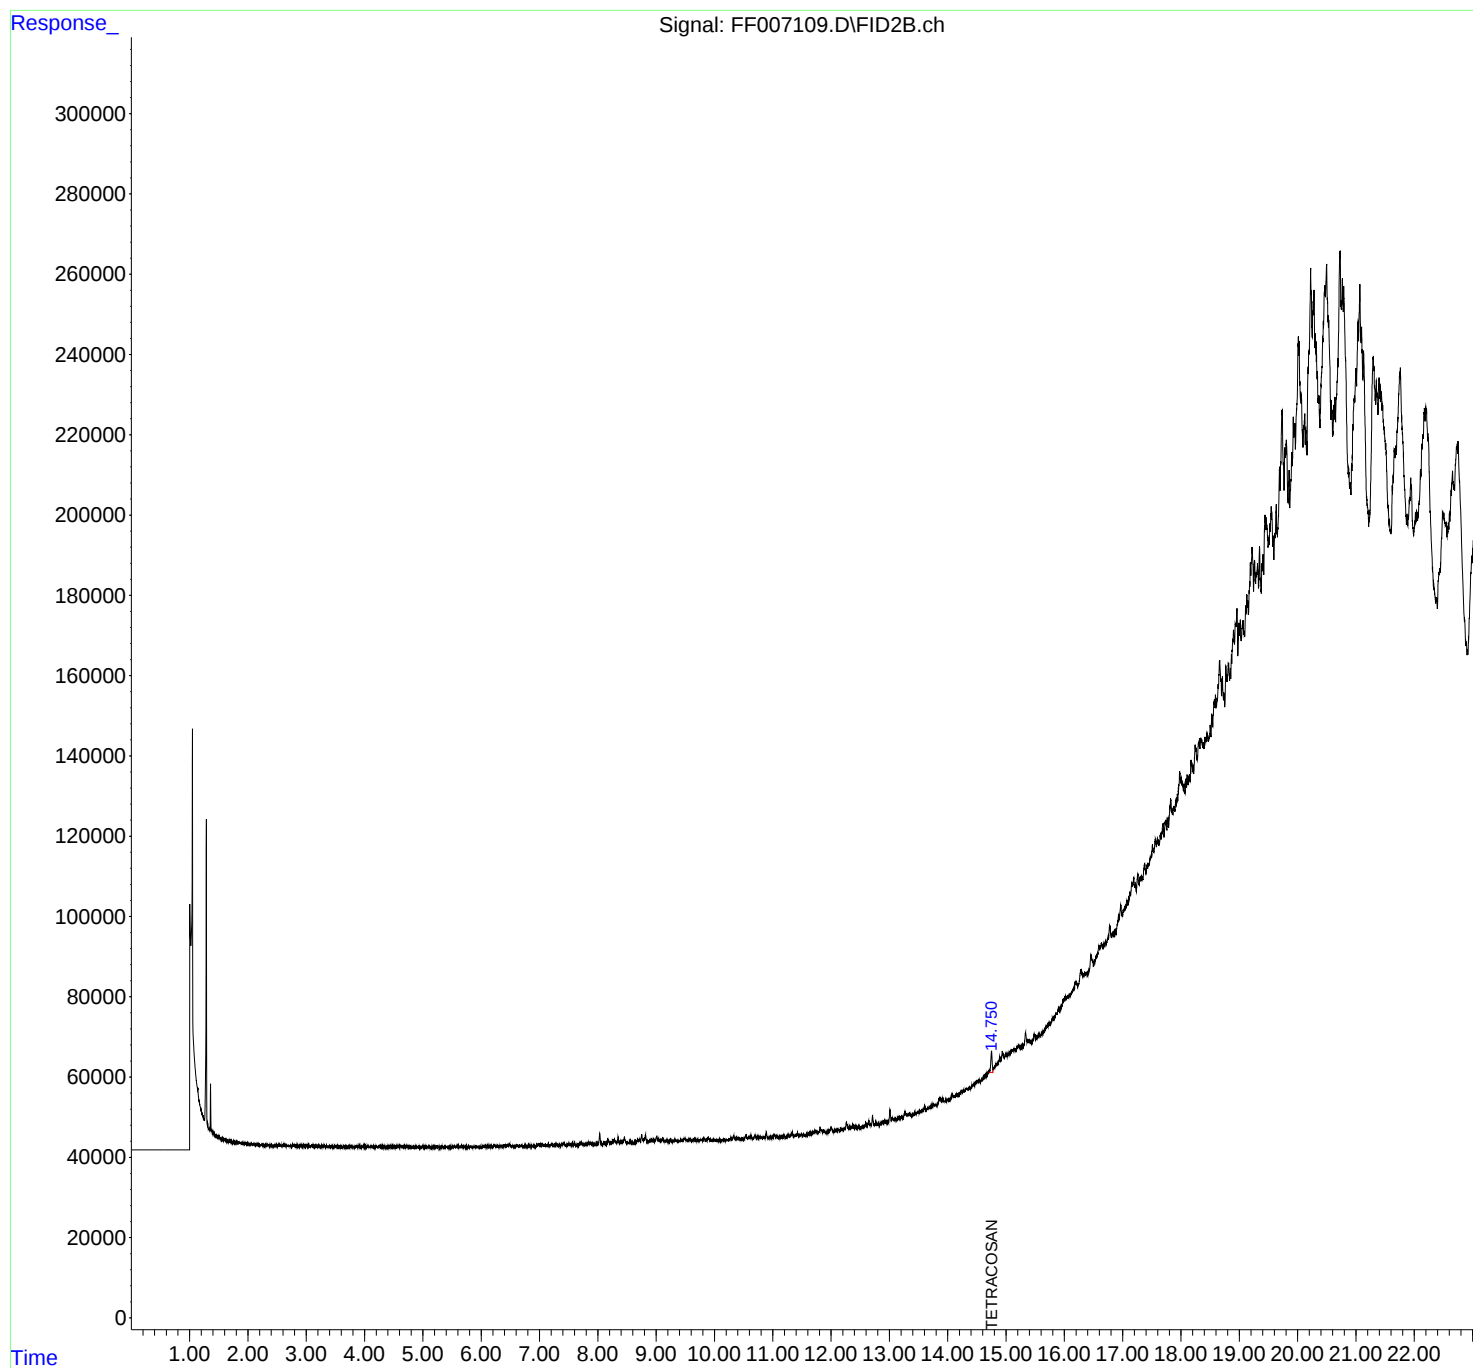

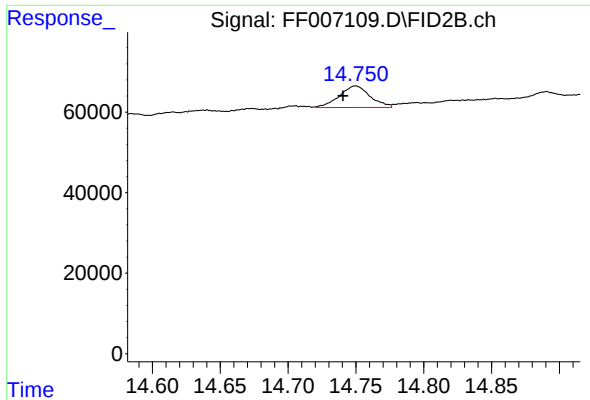

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: 0.010 min
Response: 84600
Conc: 0.72 ug/ml m

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

Ankita
6/25/2020 8:05:34 AM