

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062322\
 Data File : FF010827.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2022 09:21
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 01:04:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.714	91503	0.724 ug/ml
13) N-TRIACONTANE	17.879	95023	0.775 ug/ml
14) N-DOTRIACONTANE	18.715	213182	1.757 ug/ml
16) N-HEXATRIACONTANE	20.278f	110114	1.280 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062322\
Data File : FF010827.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2022 09:21
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:04:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

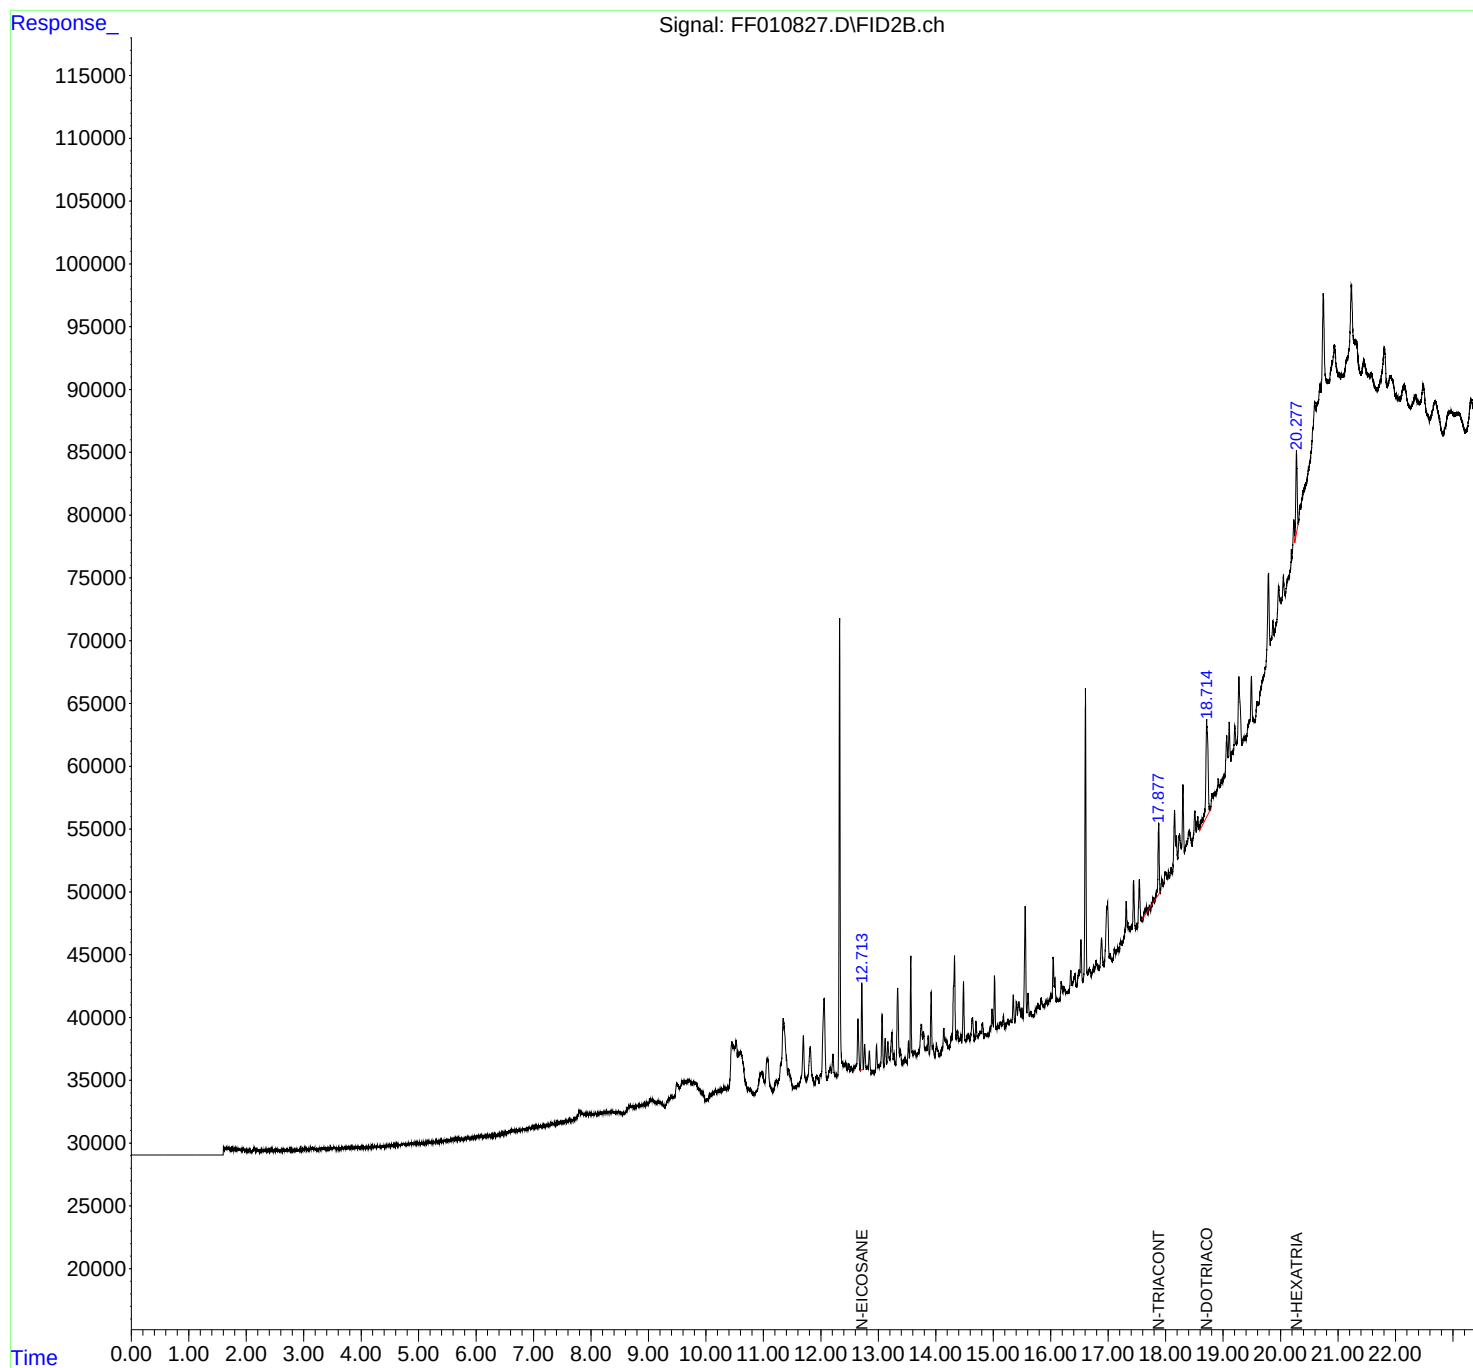


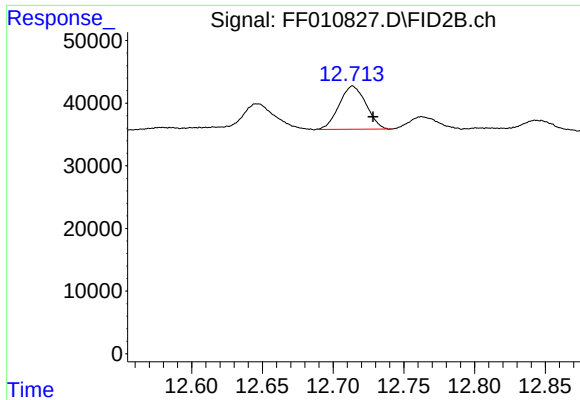

#7 N-EICOSANE


R.T.: 12.714 min
Delta R.T.: -0.014 min
Response: 91503
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

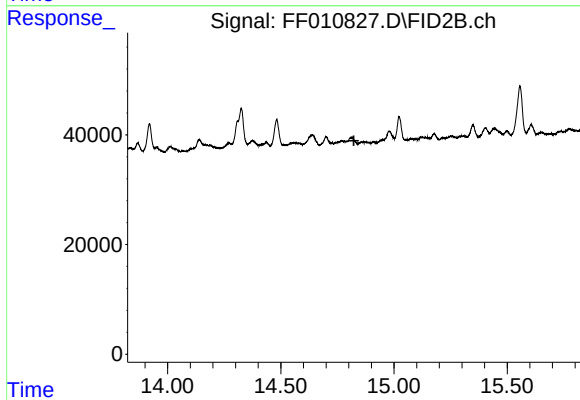


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

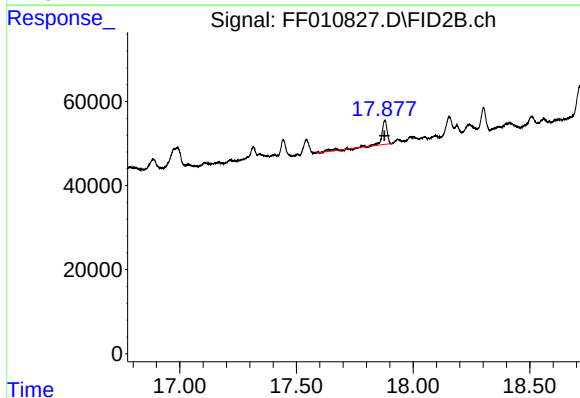


#13 N-TRIACONTANE

R.T.: 17.879 min
Delta R.T.: 0.002 min
Response: 95023
Conc: 0.78 ug/ml

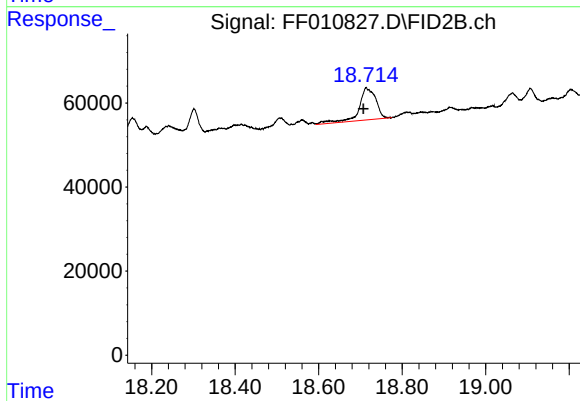

#14 N-DOTRIACONTANE

R.T.: 18.715 min
Delta R.T.: 0.007 min
Response: 213182
Conc: 1.76 ug/ml

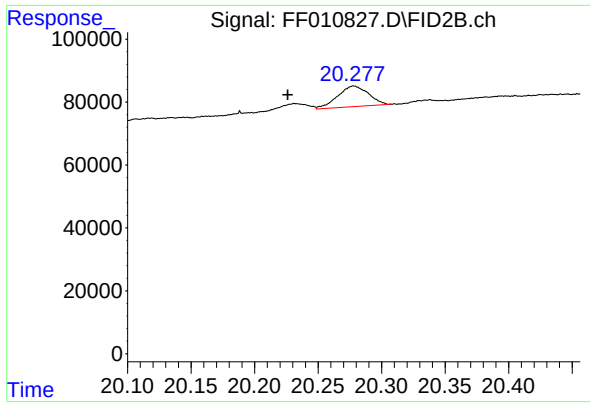

#16 N-HEXATRIACONTANE

R.T.: 20.278 min
Delta R.T.: 0.052 min
Response: 110114
Conc: 1.28 ug/ml

Instrument :

FID_F

ClientSampleId :