

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062322\
Data File : FF010834.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2022 13:48
Operator : AJ\MA
Sample : N3431-11 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:08:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.879	88092	0.719 ug/ml
14) N-DOTRIACONTANE	18.710	137973	1.137 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062322\
Data File : FF010834.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2022 13:48
Operator : AJ\MA
Sample : N3431-11 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:08:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

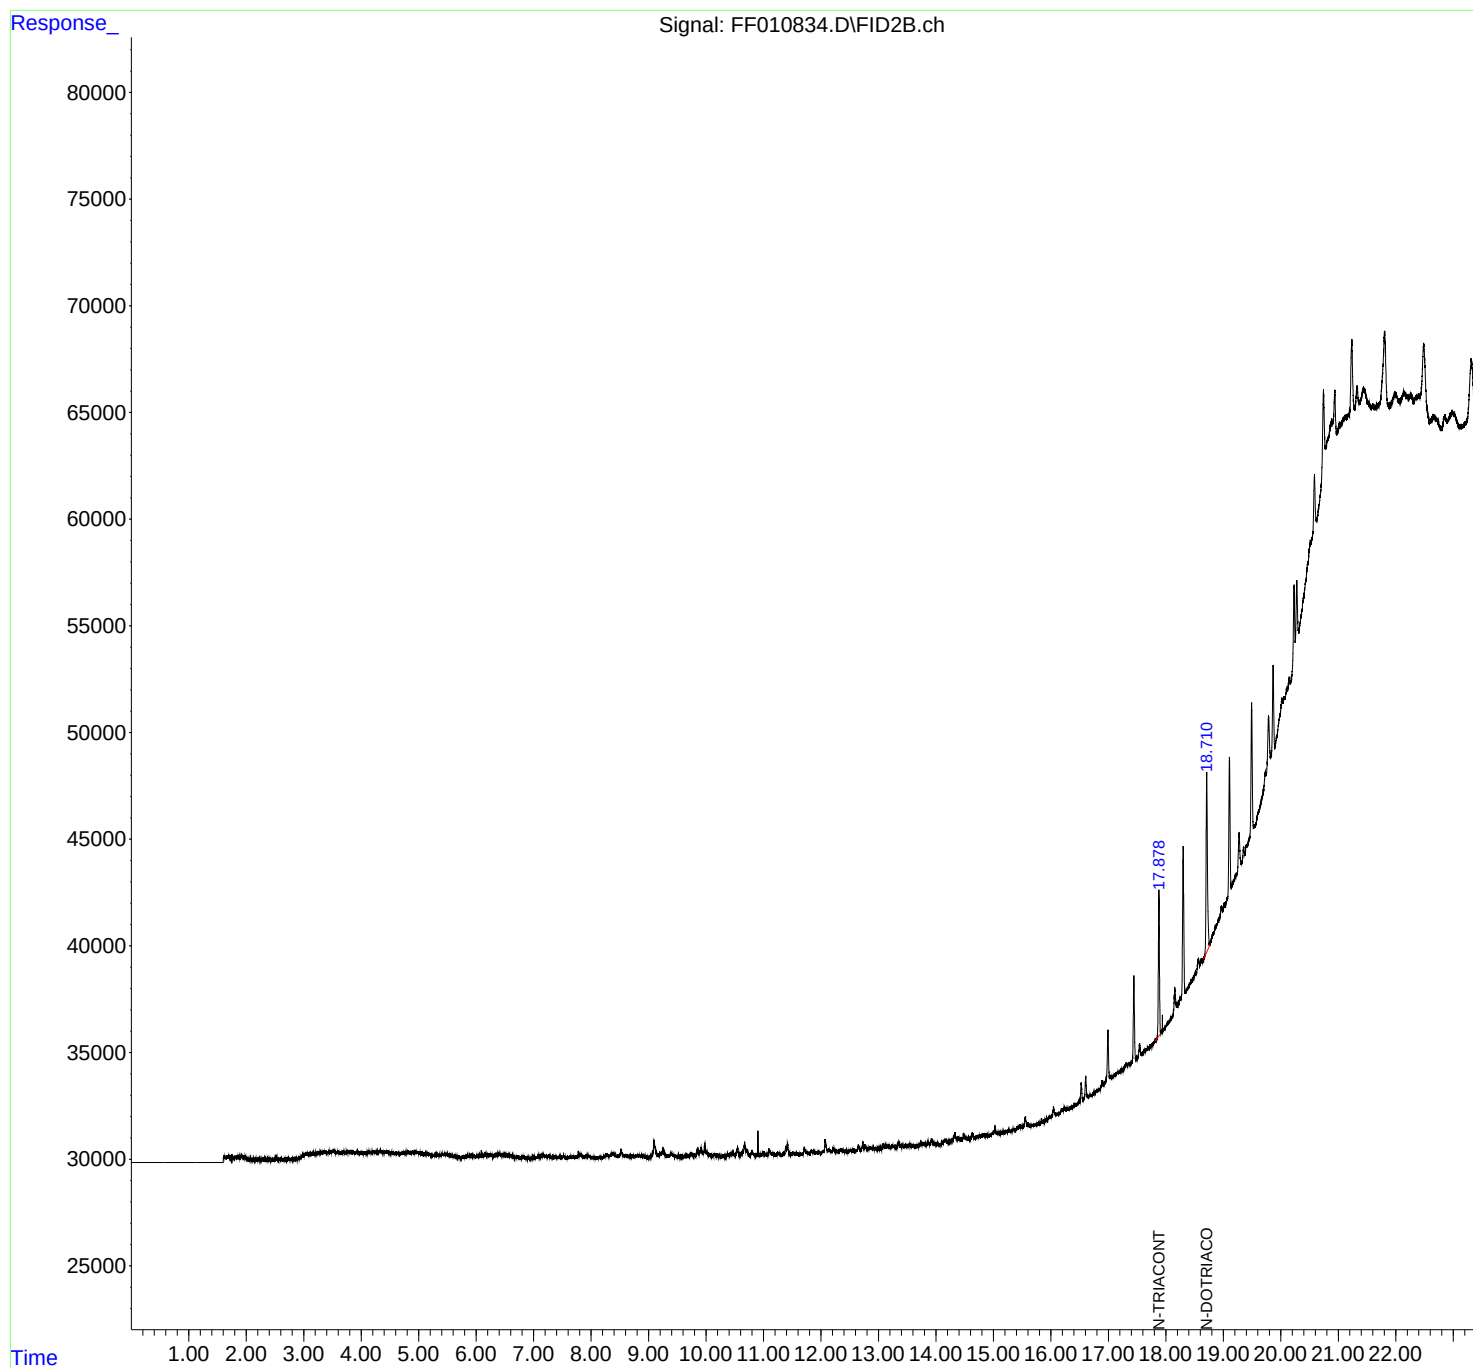


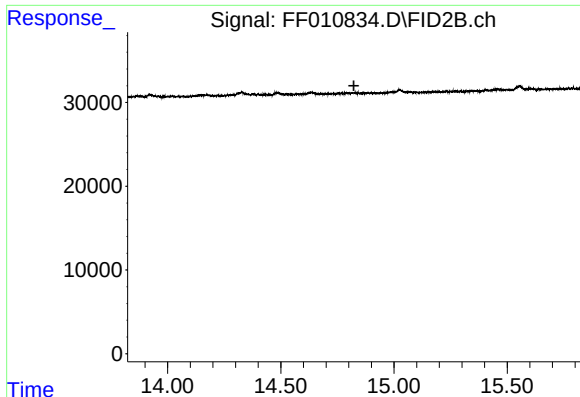

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.823 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

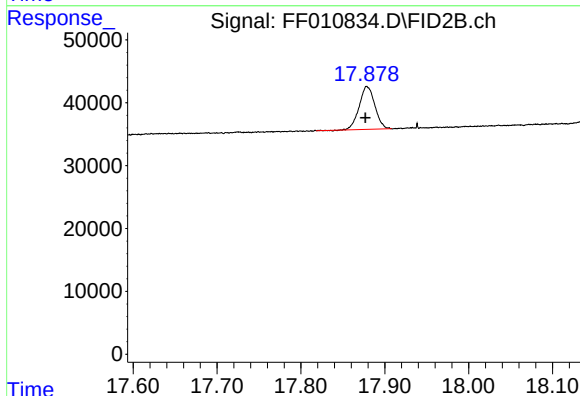

#13 N-TRIACONTANE

R.T.: 17.879 min
Delta R.T.: 0.002 min
Response: 88092
Conc: 0.72 ug/ml

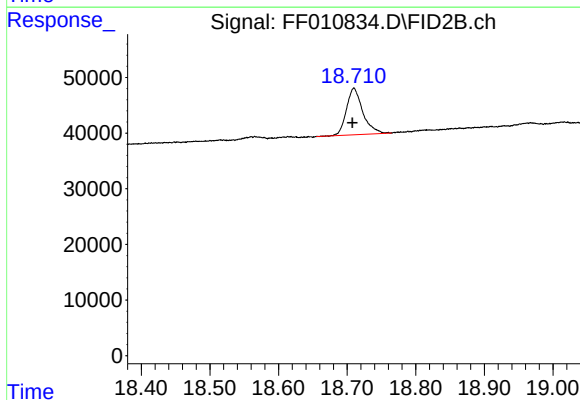

#14 N-DOTRIACONTANE

R.T.: 18.710 min
Delta R.T.: 0.003 min
Response: 137973
Conc: 1.14 ug/ml