

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
 Data File : FF012963.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 09:25
 Operator : YP\AJ
 Sample : 03355-06 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 06:37:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.998	181631	1.555 ug/ml
Target Compounds			
7) N-EICOSANE	12.940	1243119	9.077 ug/ml
8) N-DOCOSANE	14.107	128553	0.972 ug/ml
10) N-TETRACOSANE	15.162	958892	7.255 ug/ml
11) N-HEXACOSANE	16.192	45773	0.354 ug/ml
12) N-OCTACOSANE	17.174	234633	1.831 ug/ml
13) N-TRIACONTANE	18.010	136583	1.059 ug/ml
14) N-DOTRIACONTANE	18.839	354442	2.804 ug/ml
15) N-TETRATRIACONTANE	19.622	169407	1.426 ug/ml
16) N-HEXATRIACONTANE	20.432	50682	0.422 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012963.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 09:25
Operator : YP\AJ
Sample : 03355-06 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 06:37:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

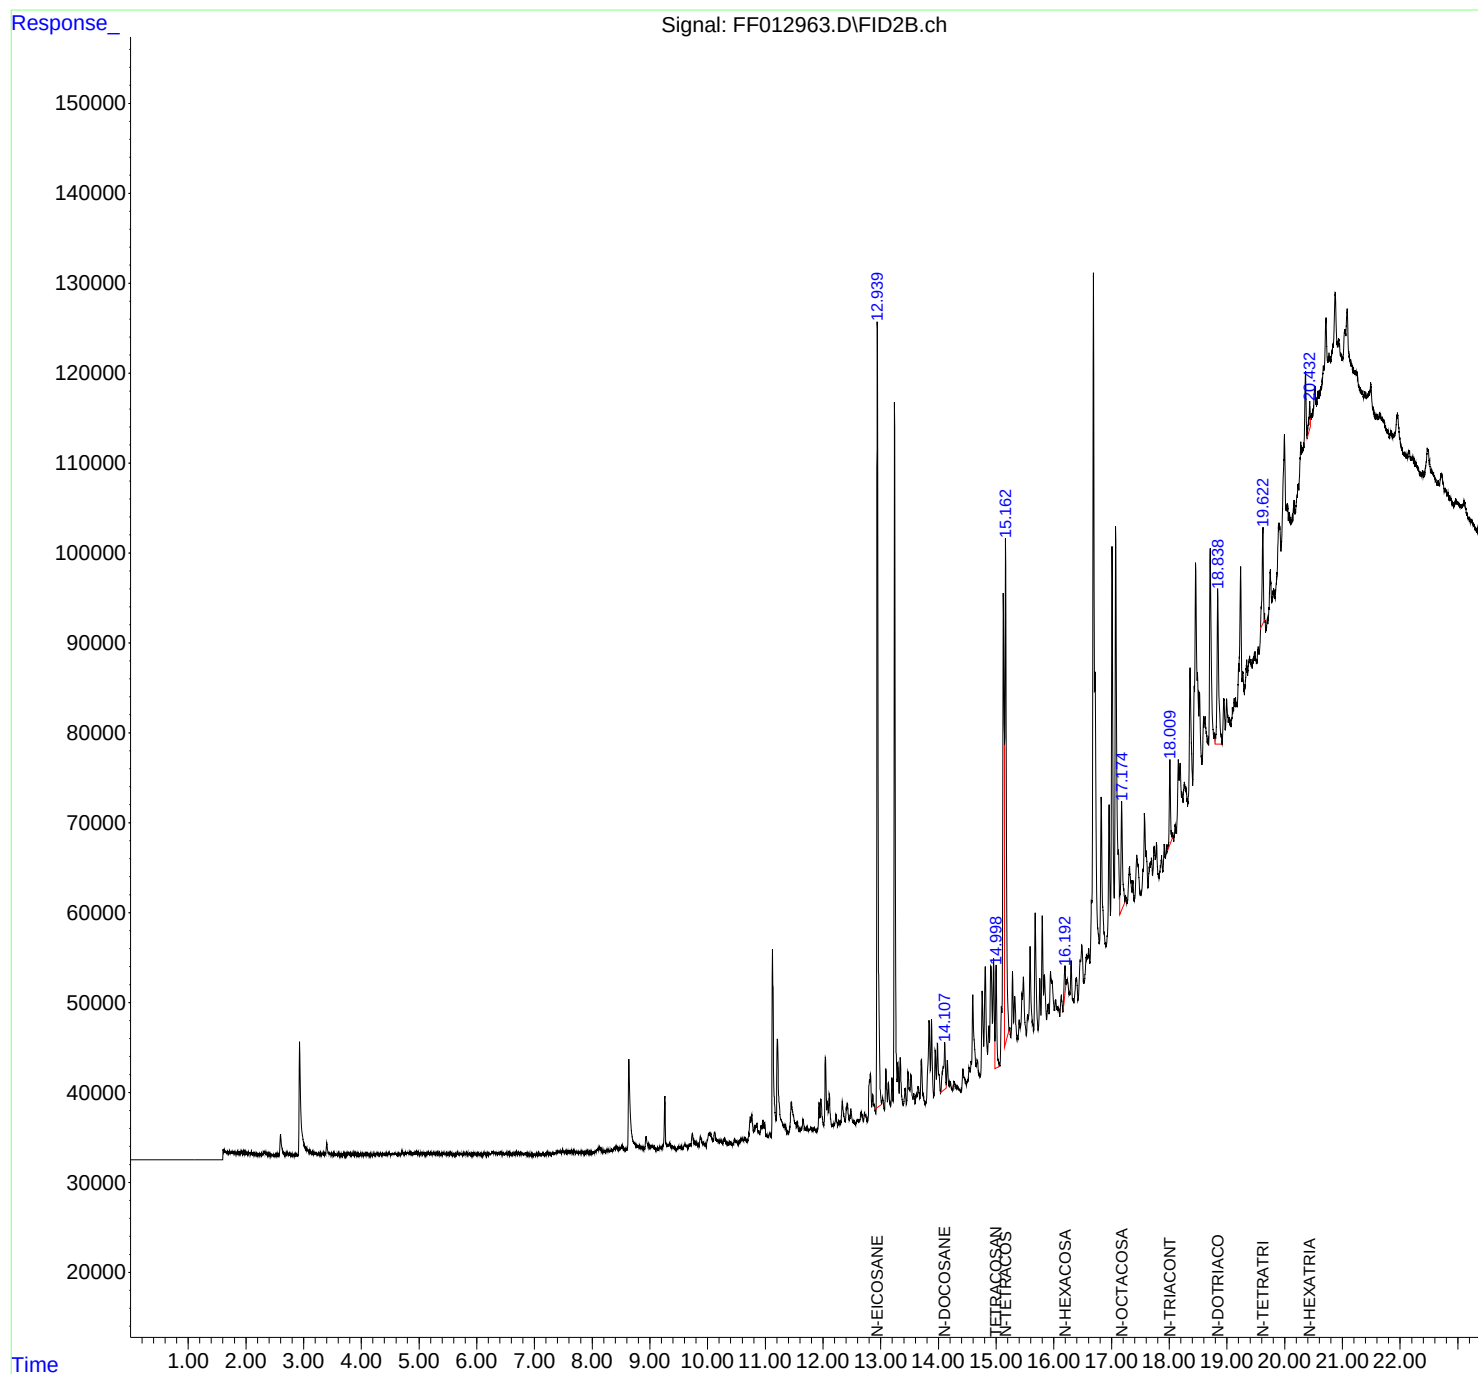


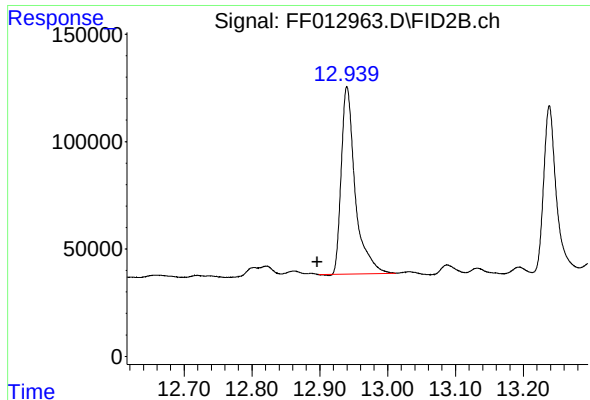

#7 N-EICOSANE


R.T.: 12.940 min
Delta R.T.: 0.044 min
Response: 1243119
Conc: 9.08 ug/ml

Instrument :
FID_F
ClientSampleId :

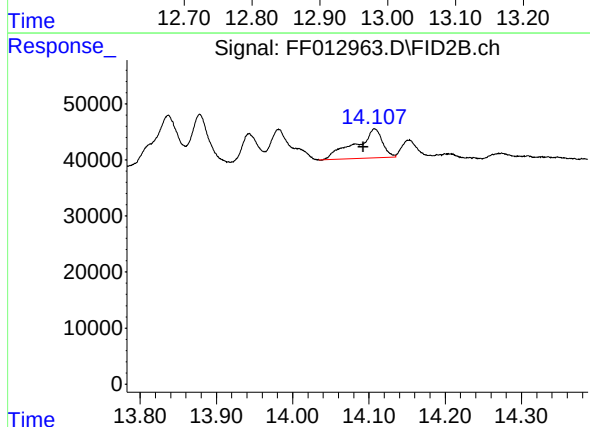


#8 N-DOCOSANE

R.T.: 14.107 min
Delta R.T.: 0.015 min
Response: 128553
Conc: 0.97 ug/ml

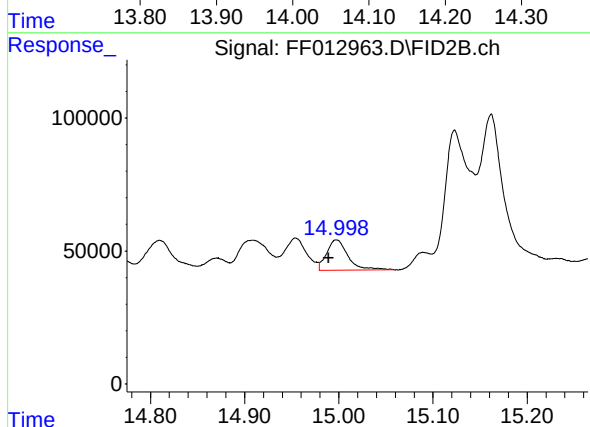


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.998 min
Delta R.T.: 0.008 min
Response: 181631
Conc: 1.56 ug/ml

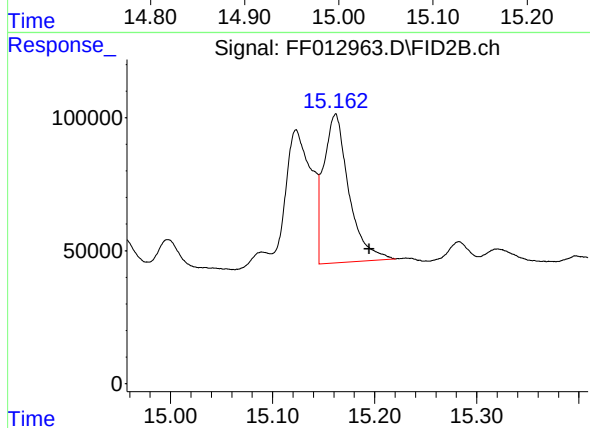

#10 N-TETRACOSANE


R.T.: 15.162 min
Delta R.T.: -0.033 min
Response: 958892
Conc: 7.26 ug/ml

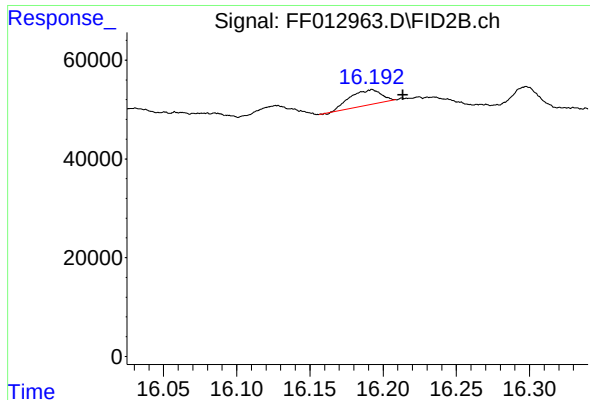

#11 N-HEXACOSANE


R.T.: 16.192 min
Delta R.T.: -0.021 min
Response: 45773
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

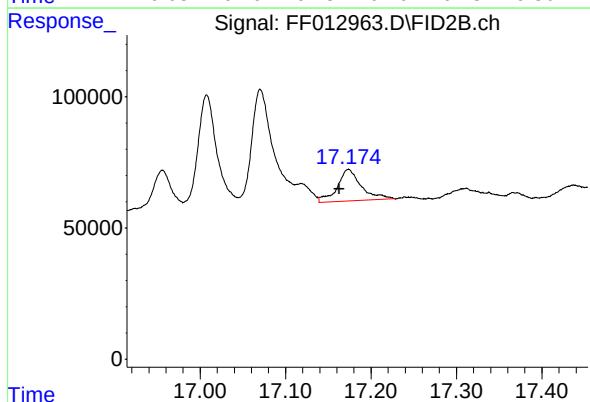


#12 N-OCTACOSANE

R.T.: 17.174 min
Delta R.T.: 0.011 min
Response: 234633
Conc: 1.83 ug/ml

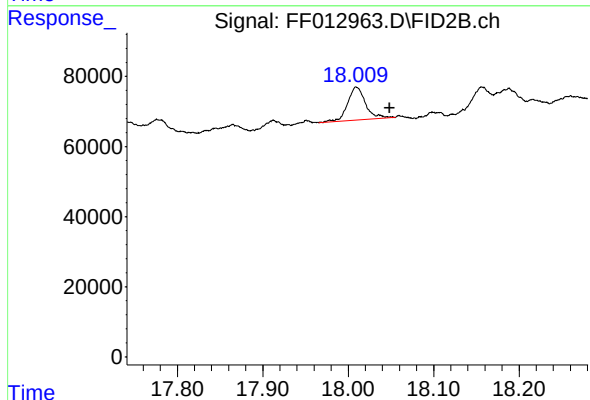


#13 N-TRIACONTANE

R.T.: 18.010 min
Delta R.T.: -0.039 min
Response: 136583
Conc: 1.06 ug/ml

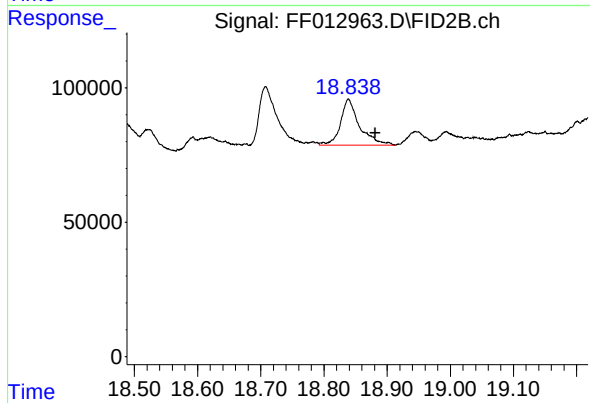

#14 N-DOTRIACONTANE


R.T.: 18.839 min
Delta R.T.: -0.043 min
Response: 354442
Conc: 2.80 ug/ml

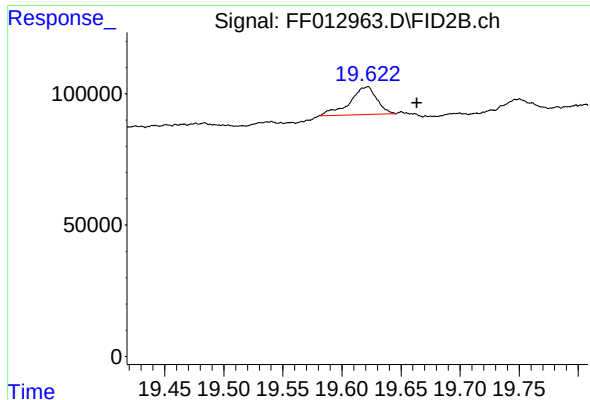

#15 N-TETRATRIACONTANE

R.T.: 19.622 min
Delta R.T.: -0.042 min
Response: 169407
Conc: 1.43 ug/ml

Instrument :
FID_F
ClientSampleId :

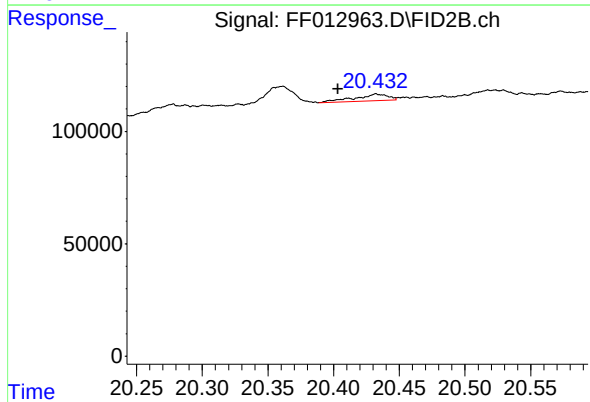

#16 N-HEXATRIACONTANE

R.T.: 20.432 min
Delta R.T.: 0.029 min
Response: 50682
Conc: 0.42 ug/ml