

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
 Data File : FF012965.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 10:23
 Operator : YP\AJ
 Sample : 03355-10 5X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 06:37:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.954	305647	2.617 ug/ml
Target Compounds			
7) N-EICOSANE	12.941	825431	6.027 ug/ml
10) N-TETRACOSANE	15.165	596512	4.513 ug/ml
11) N-HEXACOSANE	16.191	211636	1.638 ug/ml
12) N-OCTACOSANE	17.178	78527	0.613 ug/ml
13) N-TRIACONTANE	18.009	104312	0.809 ug/ml
14) N-DOTRIACONTANE	18.835	299003	2.366 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012965.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 10:23
Operator : YP\AJ
Sample : 03355-10 5X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 06:37:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

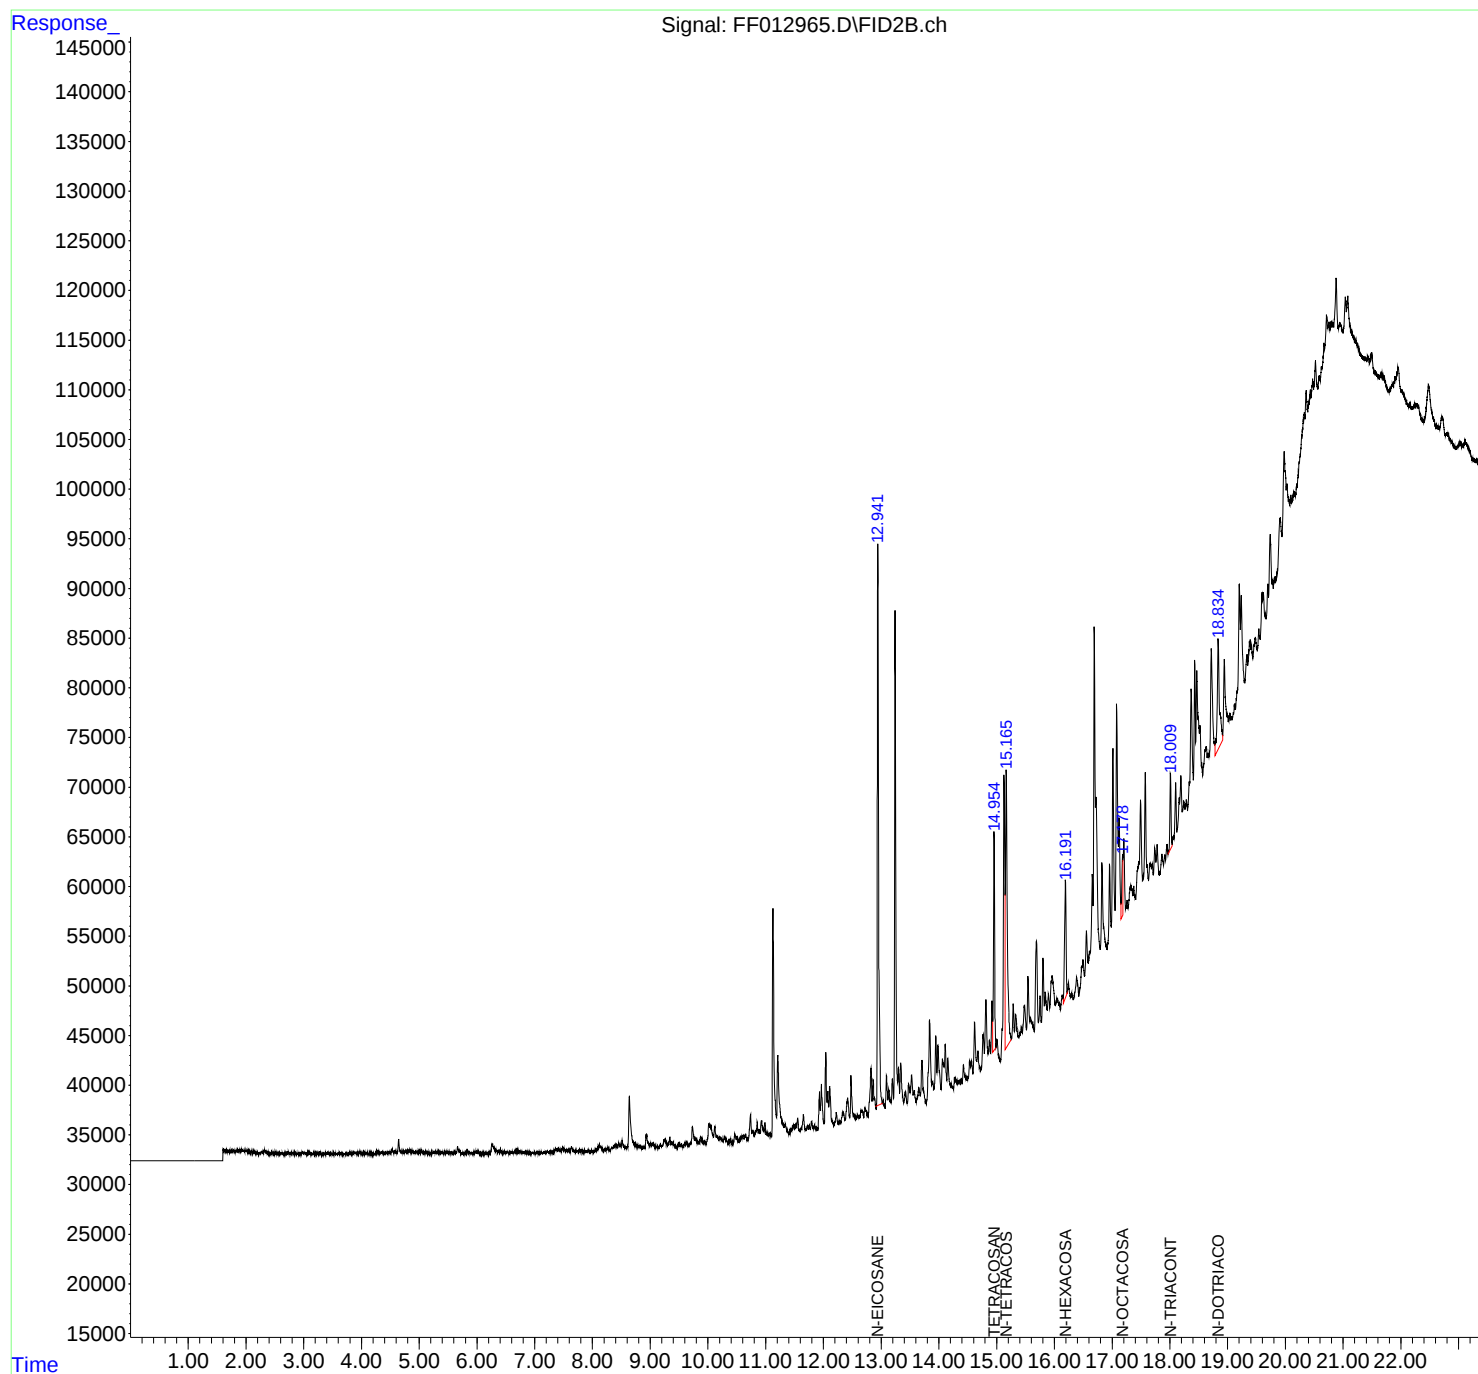


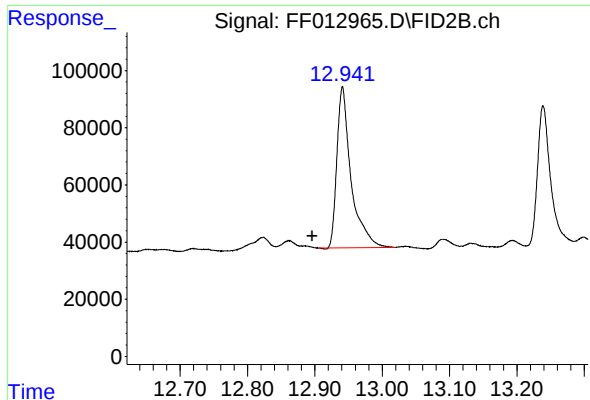

#7 N-EICOSANE


R.T.: 12.941 min
Delta R.T.: 0.045 min
Response: 825431
Conc: 6.03 ug/ml

Instrument :
FID_F
ClientSampleId :

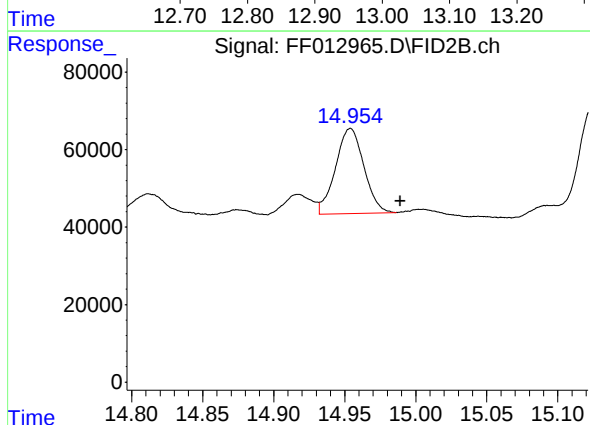


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.954 min
Delta R.T.: -0.035 min
Response: 305647
Conc: 2.62 ug/ml

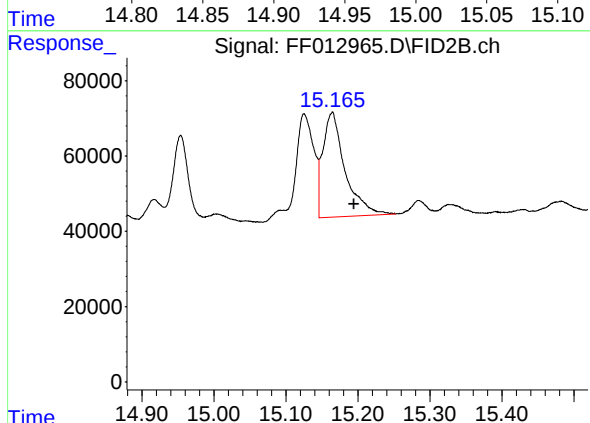


#10 N-TETRACOSANE

R.T.: 15.165 min
Delta R.T.: -0.030 min
Response: 596512
Conc: 4.51 ug/ml

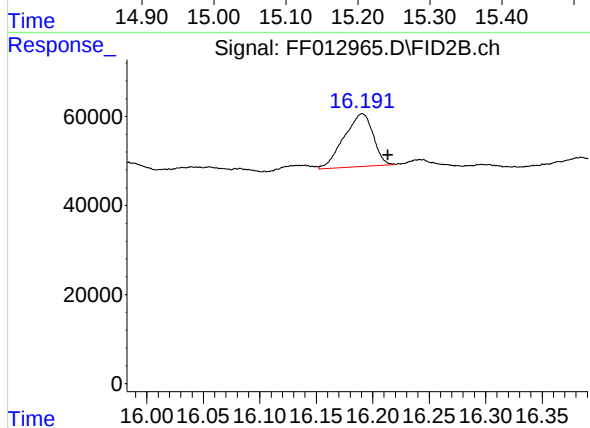

#11 N-HEXACOSANE


R.T.: 16.191 min
Delta R.T.: -0.023 min
Response: 211636
Conc: 1.64 ug/ml

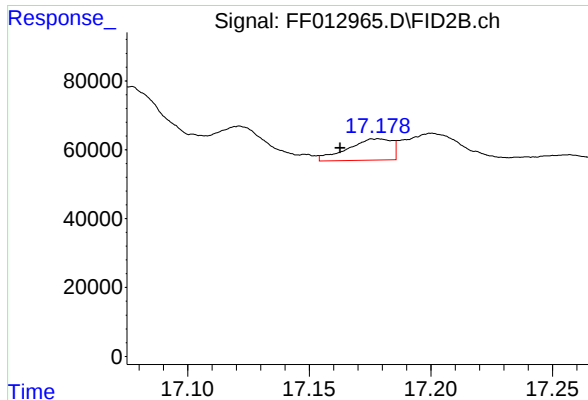

#12 N-OCTACOSANE


R.T.: 17.178 min
Delta R.T.: 0.015 min
Response: 78527
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

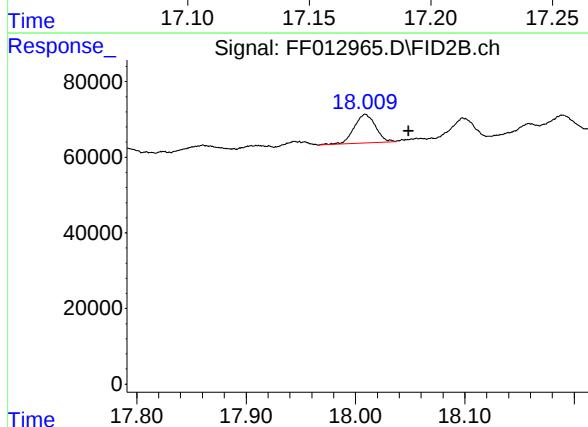

#13 N-TRIACONTANE

R.T.: 18.009 min
Delta R.T.: -0.040 min
Response: 104312
Conc: 0.81 ug/ml

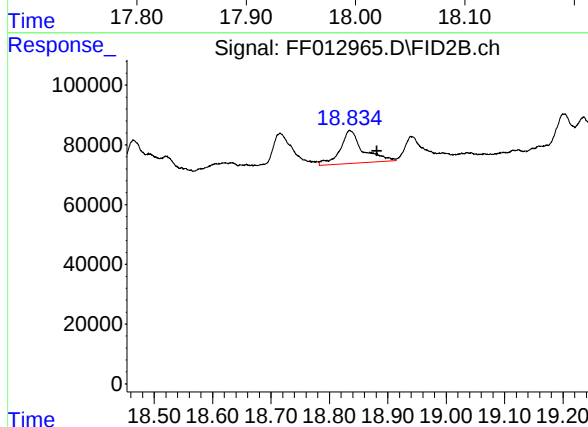

#14 N-DOTRIACONTANE

R.T.: 18.835 min
Delta R.T.: -0.046 min
Response: 299003
Conc: 2.37 ug/ml