

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
 Data File : FF012967.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 11:21
 Operator : YP\AJ
 Sample : 03355-14 5X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 06:38:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.953	347120	2.972 ug/ml
Target Compounds			
7) N-EICOSANE	12.861	90090	0.658 ug/ml
8) N-DOCOSANE	14.106	147829	1.118 ug/ml
10) N-TETRACOSANE	15.162	836069	6.326 ug/ml
11) N-HEXACOSANE	16.177	43037	0.333 ug/ml
12) N-OCTACOSANE	17.173	137044	1.069 ug/ml
13) N-TRIACONTANE	18.041	24696	0.192 ug/ml
14) N-DOTRIACONTANE	18.837	256167	2.027 ug/ml
15) N-TETRATRIACONTANE	19.695	60458	0.509 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012967.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 11:21
Operator : YP\AJ
Sample : 03355-14 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 06:38:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

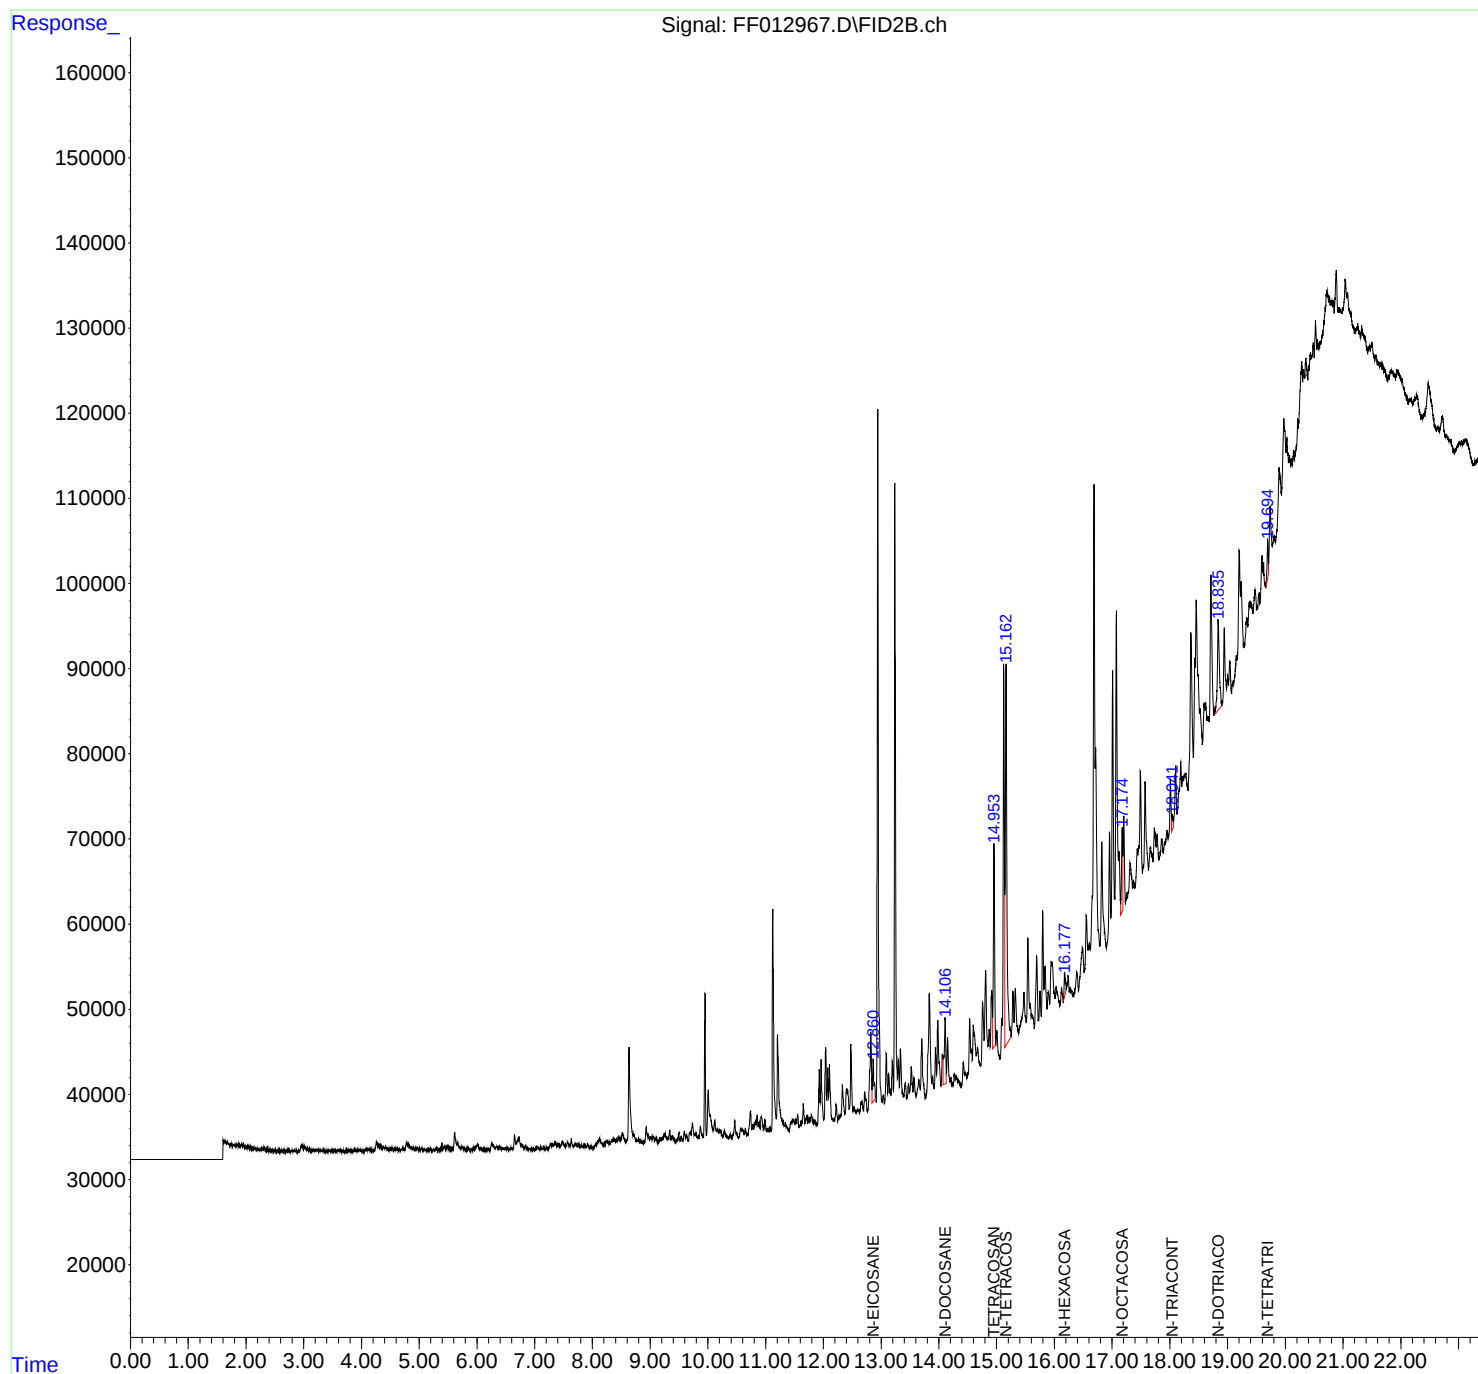


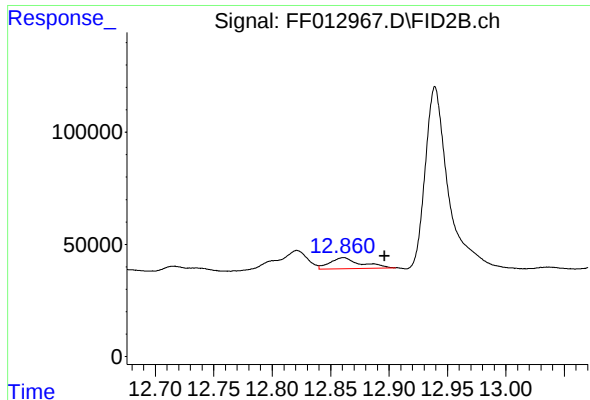

#7 N-EICOSANE


R.T.: 12.861 min
Delta R.T.: -0.035 min
Response: 90090
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

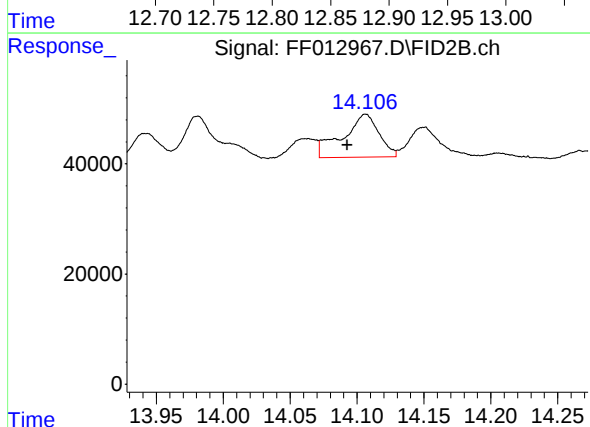


#8 N-DOCOSANE

R.T.: 14.106 min
Delta R.T.: 0.014 min
Response: 147829
Conc: 1.12 ug/ml

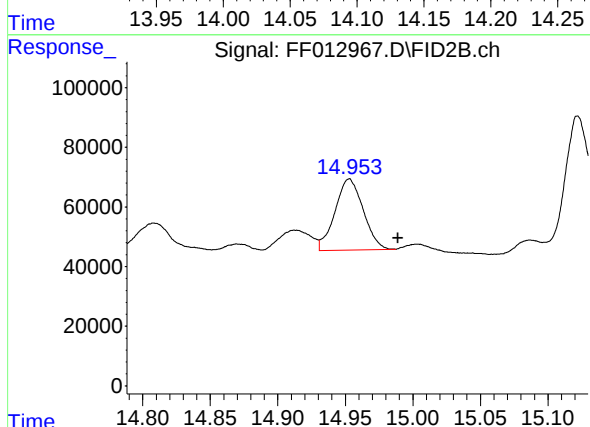


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.953 min
Delta R.T.: -0.036 min
Response: 347120
Conc: 2.97 ug/ml

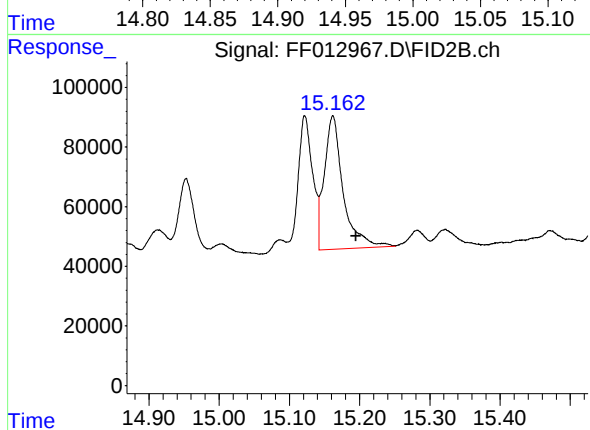

#10 N-TETRACOSANE


R.T.: 15.162 min
Delta R.T.: -0.033 min
Response: 836069
Conc: 6.33 ug/ml

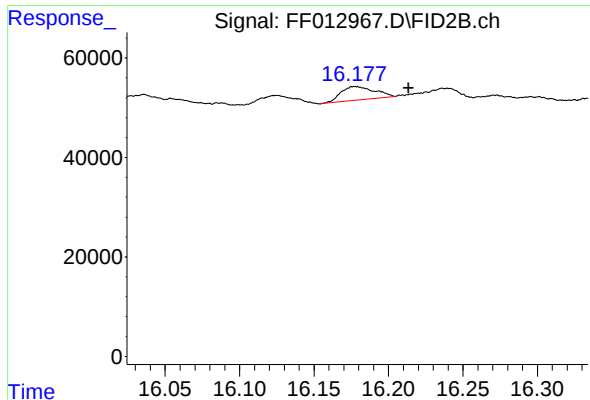

#11 N-HEXACOSANE


R.T.: 16.177 min
Delta R.T.: -0.036 min
Response: 43037
Conc: 0.33 ug/ml

Instrument :
FID_F
ClientSampleId :

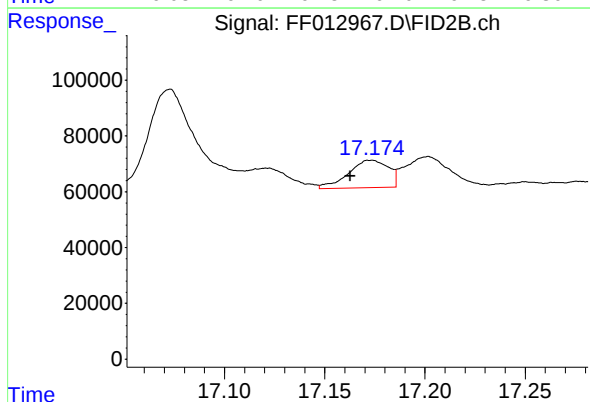


#12 N-OCTACOSANE

R.T.: 17.173 min
Delta R.T.: 0.010 min
Response: 137044
Conc: 1.07 ug/ml

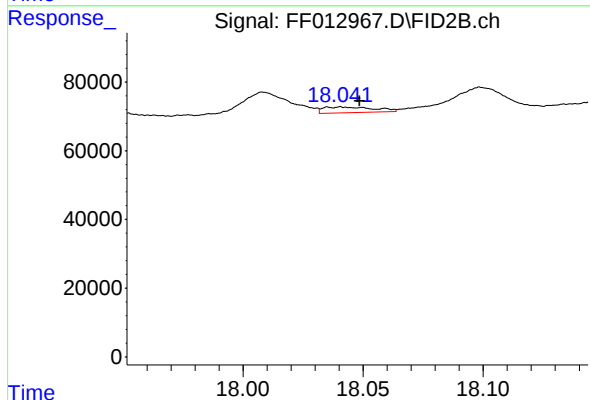


#13 N-TRIACONTANE

R.T.: 18.041 min
Delta R.T.: -0.008 min
Response: 24696
Conc: 0.19 ug/ml

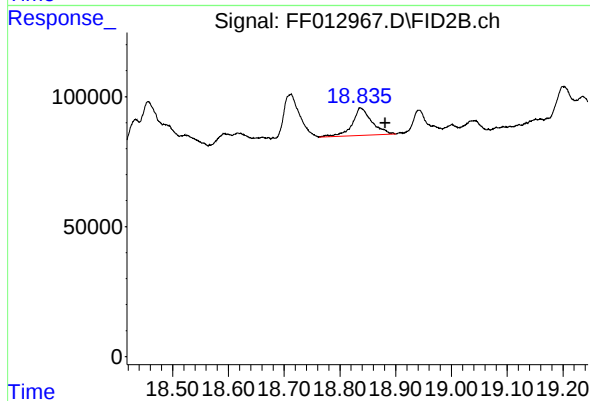

#14 N-DOTRIACONTANE

R.T.: 18.837 min
Delta R.T.: -0.045 min
Response: 256167
Conc: 2.03 ug/ml

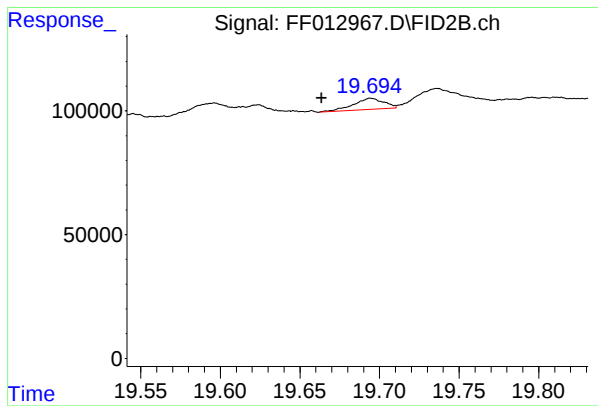

#15 N-TETRATRIACONTANE

R.T.: 19.695 min
Delta R.T.: 0.031 min
Response: 60458
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :