

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
 Data File : FF012969.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 12:20
 Operator : YP\AJ
 Sample : 03357-14 100X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 06:38:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.974	69813	0.598 ug/ml
Target Compounds			
8) N-DOCOSANE	14.117	59906	0.453 ug/ml
10) N-TETRACOSANE	15.219	214501	1.623 ug/ml
11) N-HEXACOSANE	16.216	173425	1.342 ug/ml
12) N-OCTACOSANE	17.152	107809	0.841 ug/ml
14) N-DOTRIACONTANE	18.945f	131216	1.038 ug/ml
15) N-TETRATRIACONTANE	19.654	86191	0.726 ug/ml
16) N-HEXATRIACONTANE	20.437	89668	0.747 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012969.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 12:20
Operator : YP\AJ
Sample : 03357-14 100X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 06:38:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

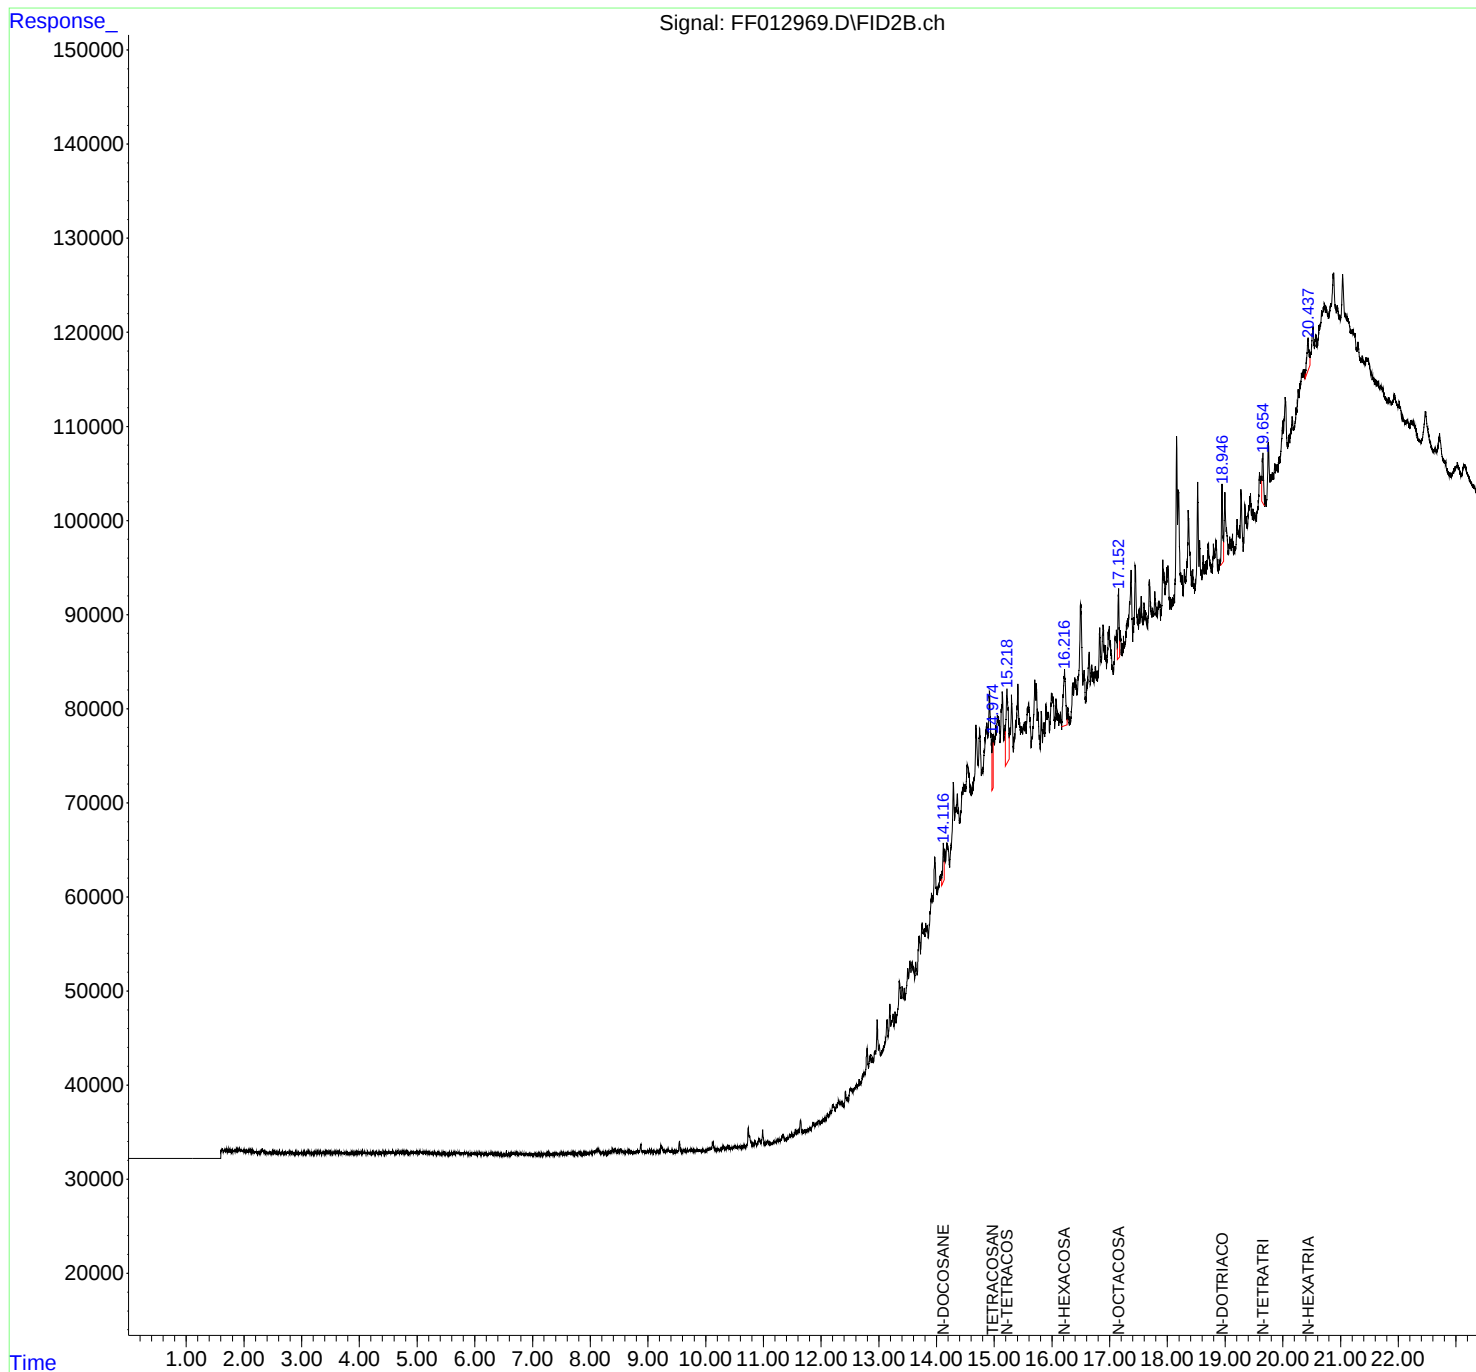


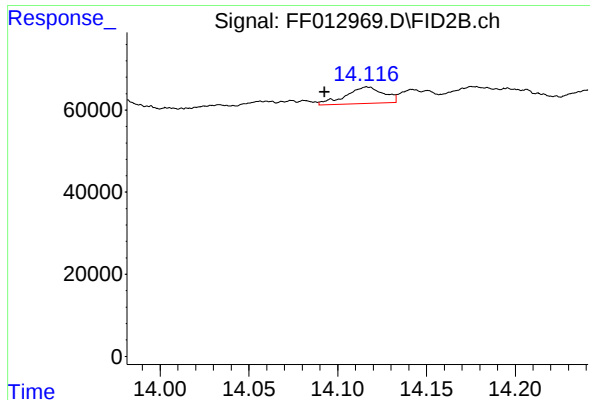

#8 N-DOCOSANE


R.T.: 14.117 min
Delta R.T.: 0.024 min
Response: 59906
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :

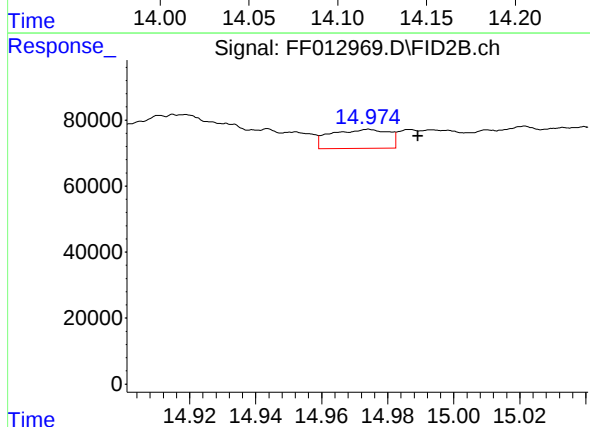


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.974 min
Delta R.T.: -0.015 min
Response: 69813
Conc: 0.60 ug/ml

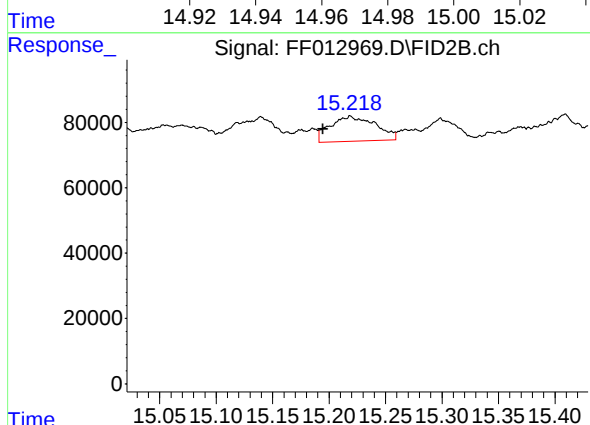


#10 N-TETRACOSANE

R.T.: 15.219 min
Delta R.T.: 0.024 min
Response: 214501
Conc: 1.62 ug/ml

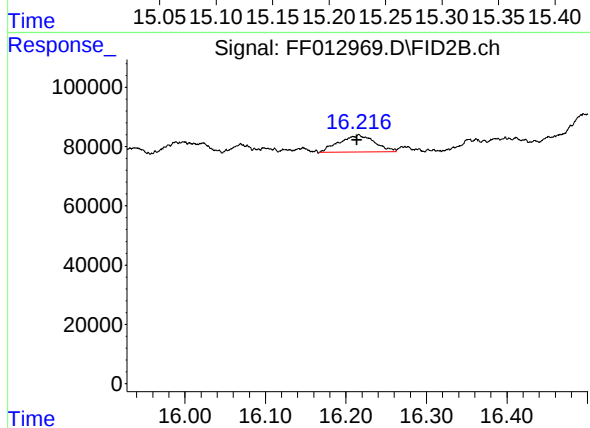

#11 N-HEXACOSANE


R.T.: 16.216 min
Delta R.T.: 0.002 min
Response: 173425
Conc: 1.34 ug/ml

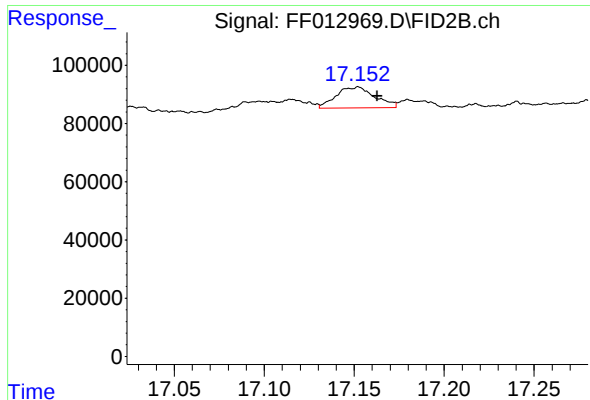

#12 N-OCTACOSANE


R.T.: 17.152 min
Delta R.T.: -0.011 min
Response: 107809
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

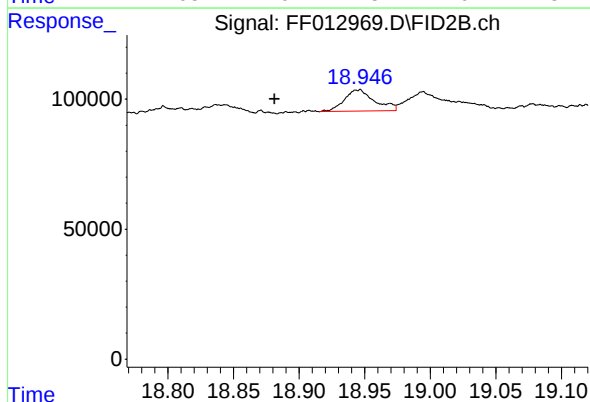


#14 N-DOTRIACONTANE

R.T.: 18.945 min
Delta R.T.: 0.064 min
Response: 131216
Conc: 1.04 ug/ml

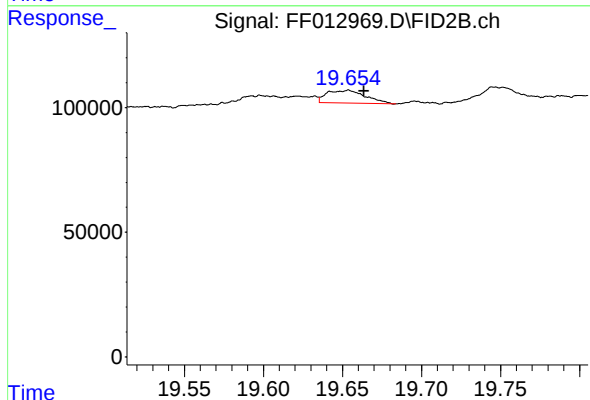

#15 N-TETRATRIACONTANE

R.T.: 19.654 min
Delta R.T.: -0.010 min
Response: 86191
Conc: 0.73 ug/ml

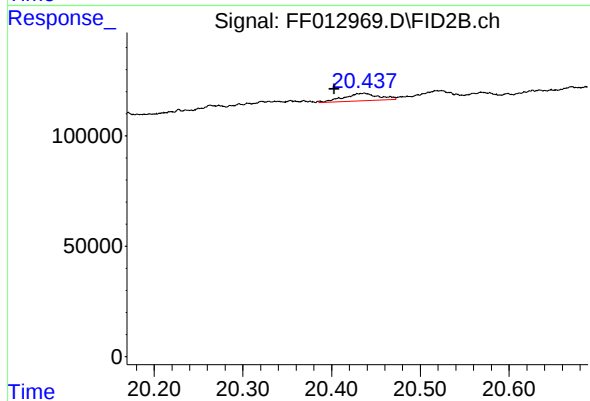

#16 N-HEXATRIACONTANE

R.T.: 20.437 min
Delta R.T.: 0.034 min
Response: 89668
Conc: 0.75 ug/ml