

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
 Data File : FF012970.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 12:49
 Operator : YP\AJ
 Sample : 03357-19 200X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 06:38:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Tue Jun 13 04:35:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	1369616	11.728 ug/ml
Target Compounds			
6) N-OCTADECANE	11.601	130728	0.952 ug/ml
7) N-EICOSANE	12.894	552930	4.037 ug/ml
8) N-DOCOSANE	14.073	1042798	7.888 ug/ml
10) N-TETRACOSANE	15.214	2601621	19.685 ug/ml
14) N-DOTRIACONTANE	18.841	45825	0.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012970.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 12:49
Operator : YP\AJ
Sample : 03357-19 200X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 06:38:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

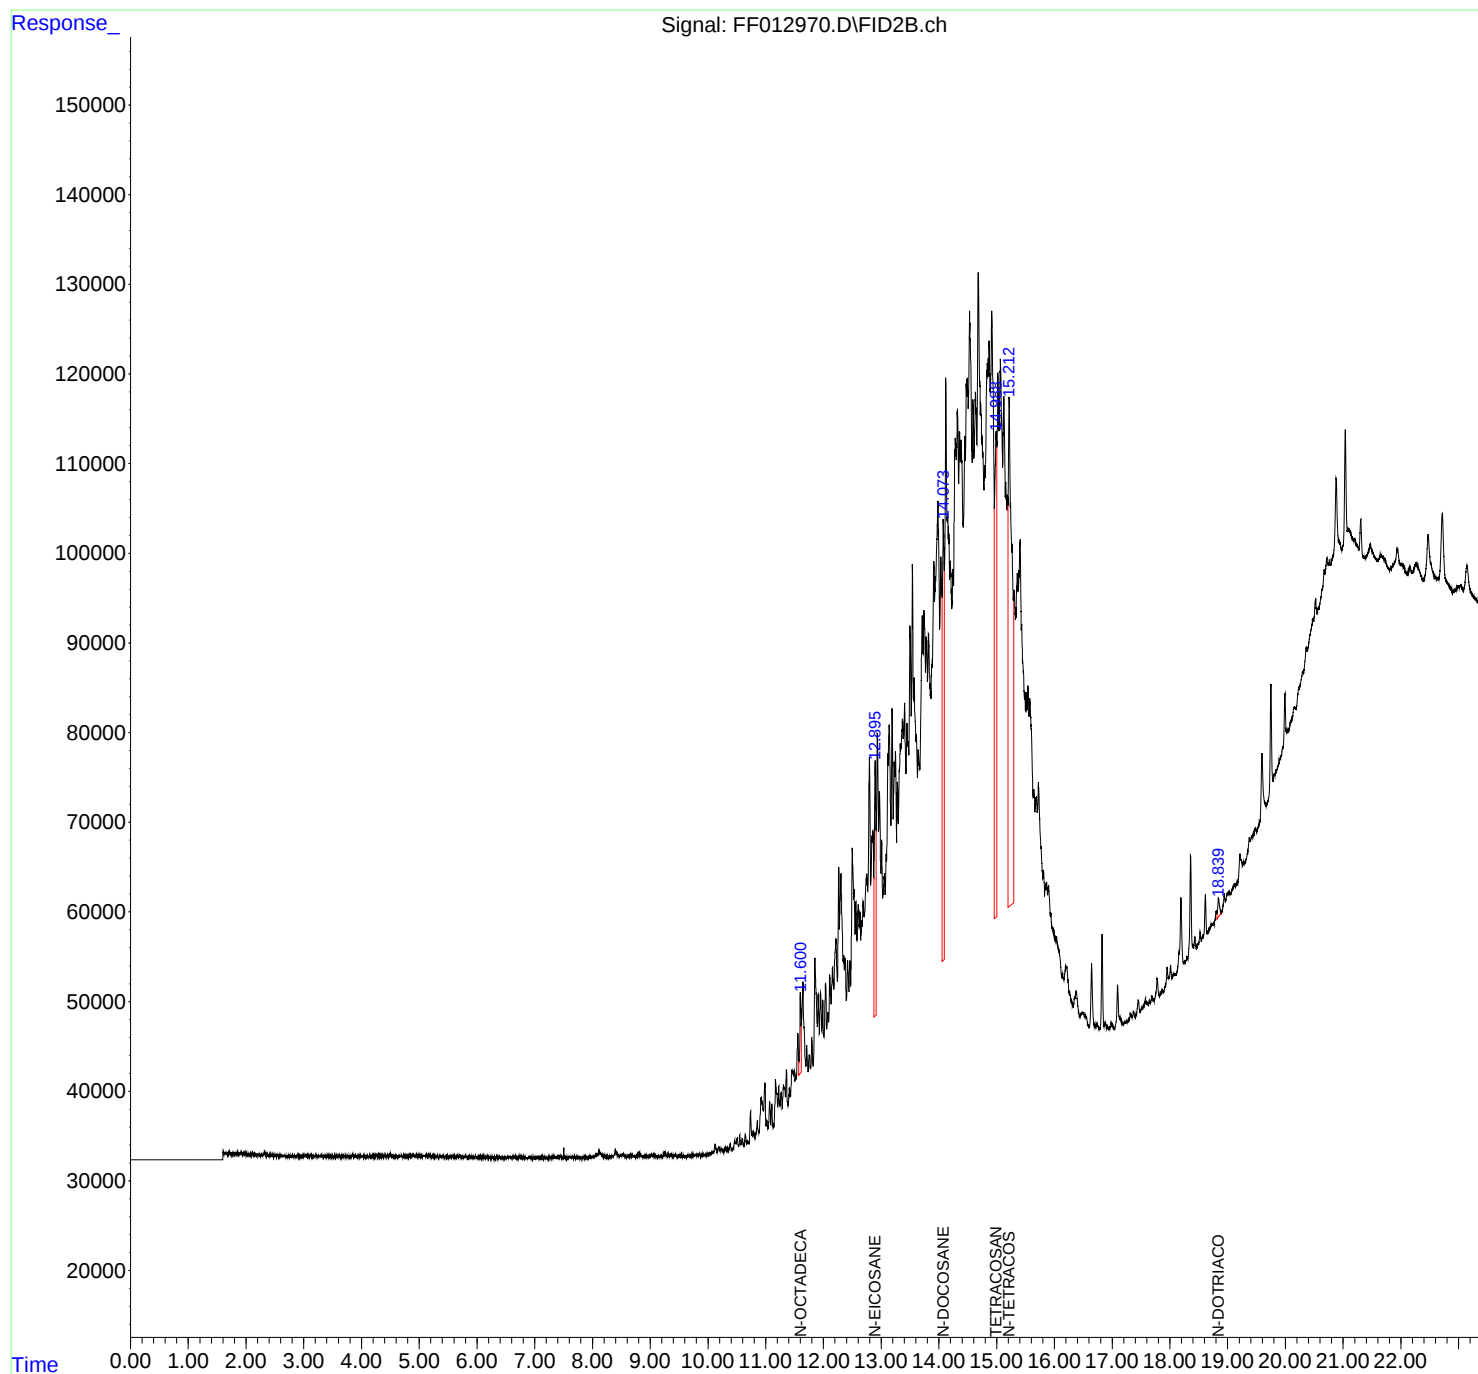


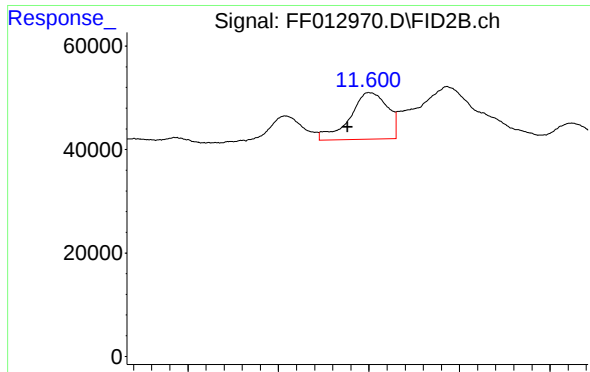

#6 N-OCTADECANE


R.T.: 11.601 min
Delta R.T.: 0.012 min
Response: 130728
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :

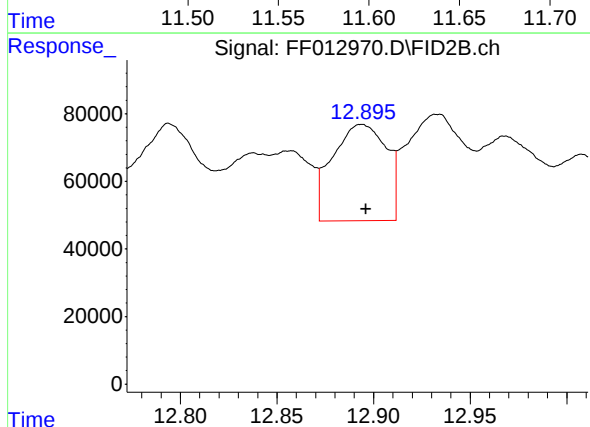


#7 N-EICOSANE

R.T.: 12.894 min
Delta R.T.: -0.003 min
Response: 552930
Conc: 4.04 ug/ml

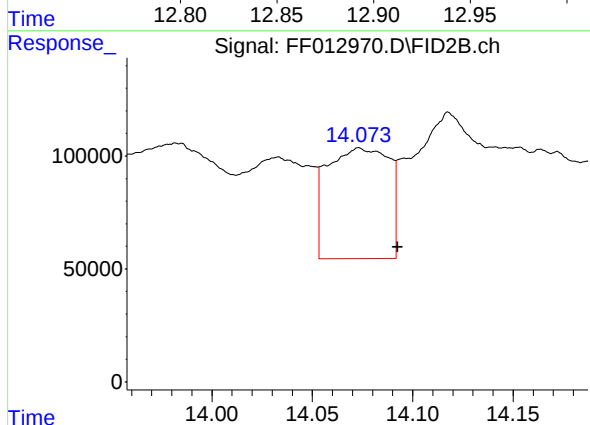


#8 N-DOCOSANE

R.T.: 14.073 min
Delta R.T.: -0.019 min
Response: 1042798
Conc: 7.89 ug/ml

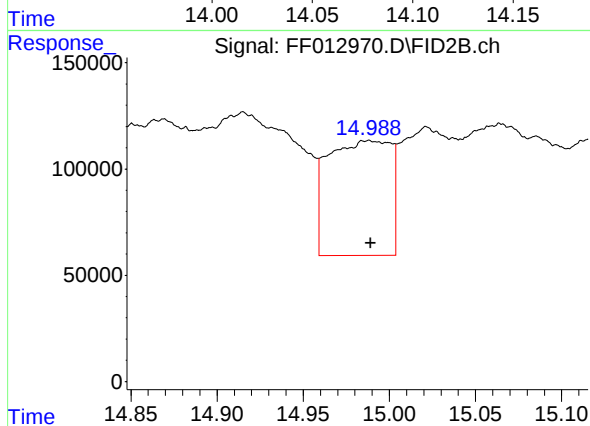

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.988 min
Delta R.T.: -0.001 min
Response: 1369616
Conc: 11.73 ug/ml

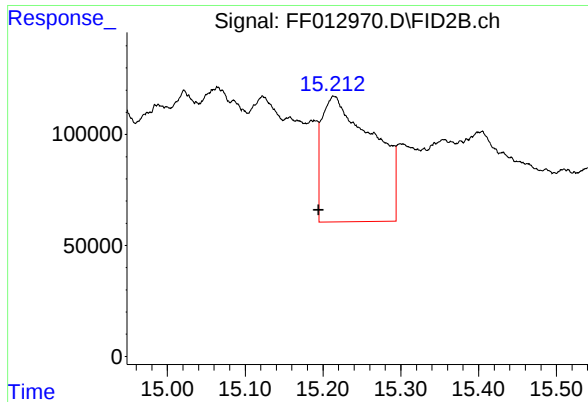

#10 N-TETRACOSANE

R.T.: 15.214 min
Delta R.T.: 0.020 min
Response: 2601621
Conc: 19.69 ug/ml

Instrument :
FID_F
ClientSampleId :

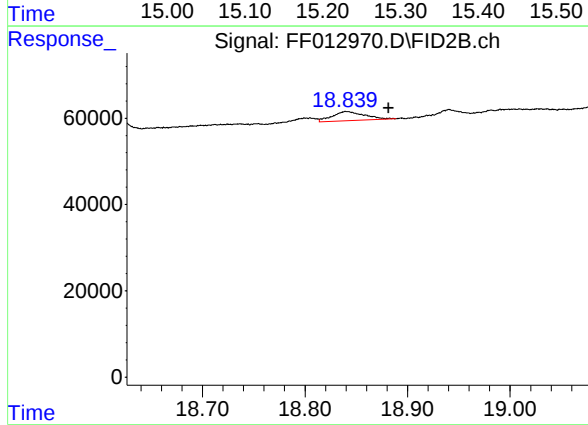

#14 N-DOTRIACONTANE

R.T.: 18.841 min
Delta R.T.: -0.041 min
Response: 45825
Conc: 0.36 ug/ml