

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012968.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 11:50
Operator : YP\AJ
Sample : 03357-04 10X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-SCAN-01-G

Integration File: autoint1.e
Quant Time: Jun 24 06:38:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.954	171634	1.470 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323\
Data File : FF012968.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 11:50
Operator : YP\AJ
Sample : 03357-04 10X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-SCAN-01-G

Integration File: autoint1.e
Quant Time: Jun 24 06:38:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Tue Jun 13 04:35:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

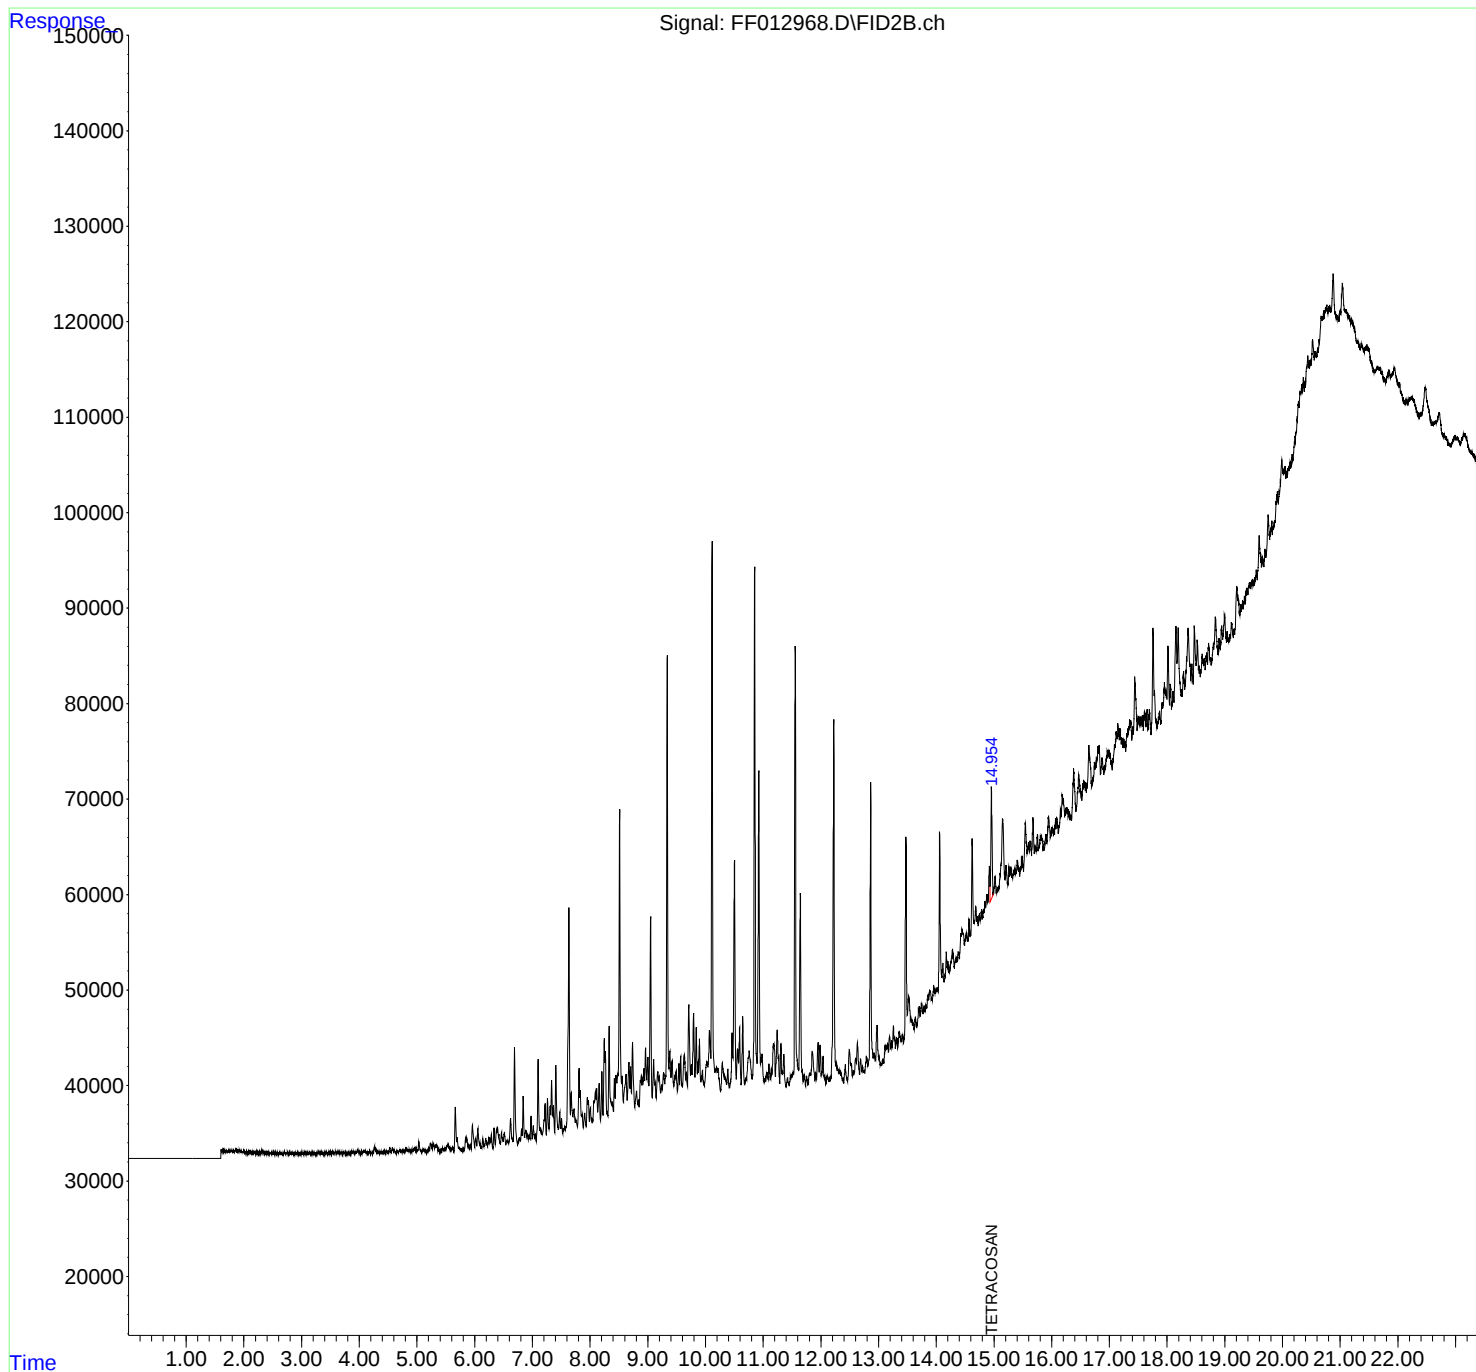

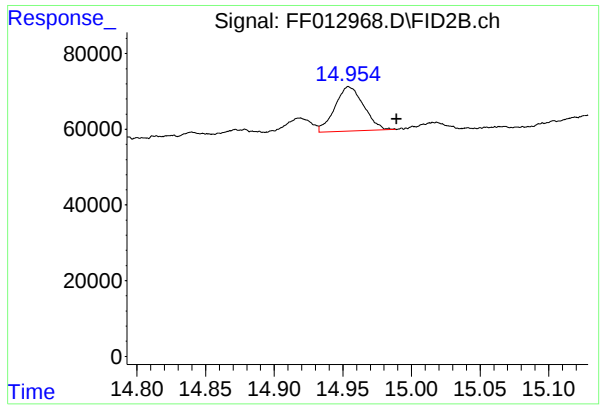

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.954 min
Delta R.T.: -0.035 min
Response: 171634
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-SCAN-01-G