

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062323\  
 Data File : FF012971.D  
 Signal(s) : FID2B.ch  
 Acq On : 23 Jun 2023 13:18  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 I.BLK

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/24/2023  
 Supervised By :Ankita Jodhani 06/26/2023

Integration File: autoint1.e  
 Quant Time: Jun 24 06:38:30 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060223.M  
 Quant Title :  
 QLast Update : Tue Jun 13 04:35:09 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.954 | 1879870  | 16.098 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF062323\  
Data File : FF012971.D  
Signal(s) : FID2B.ch  
Acq On : 23 Jun 2023 13:18  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
I.BLK


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/24/2023  
Supervised By :Ankita Jodhani 06/26/2023

Integration File: autoint1.e  
Quant Time: Jun 24 06:38:30 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060223.M  
Quant Title :  
QLast Update : Tue Jun 13 04:35:09 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

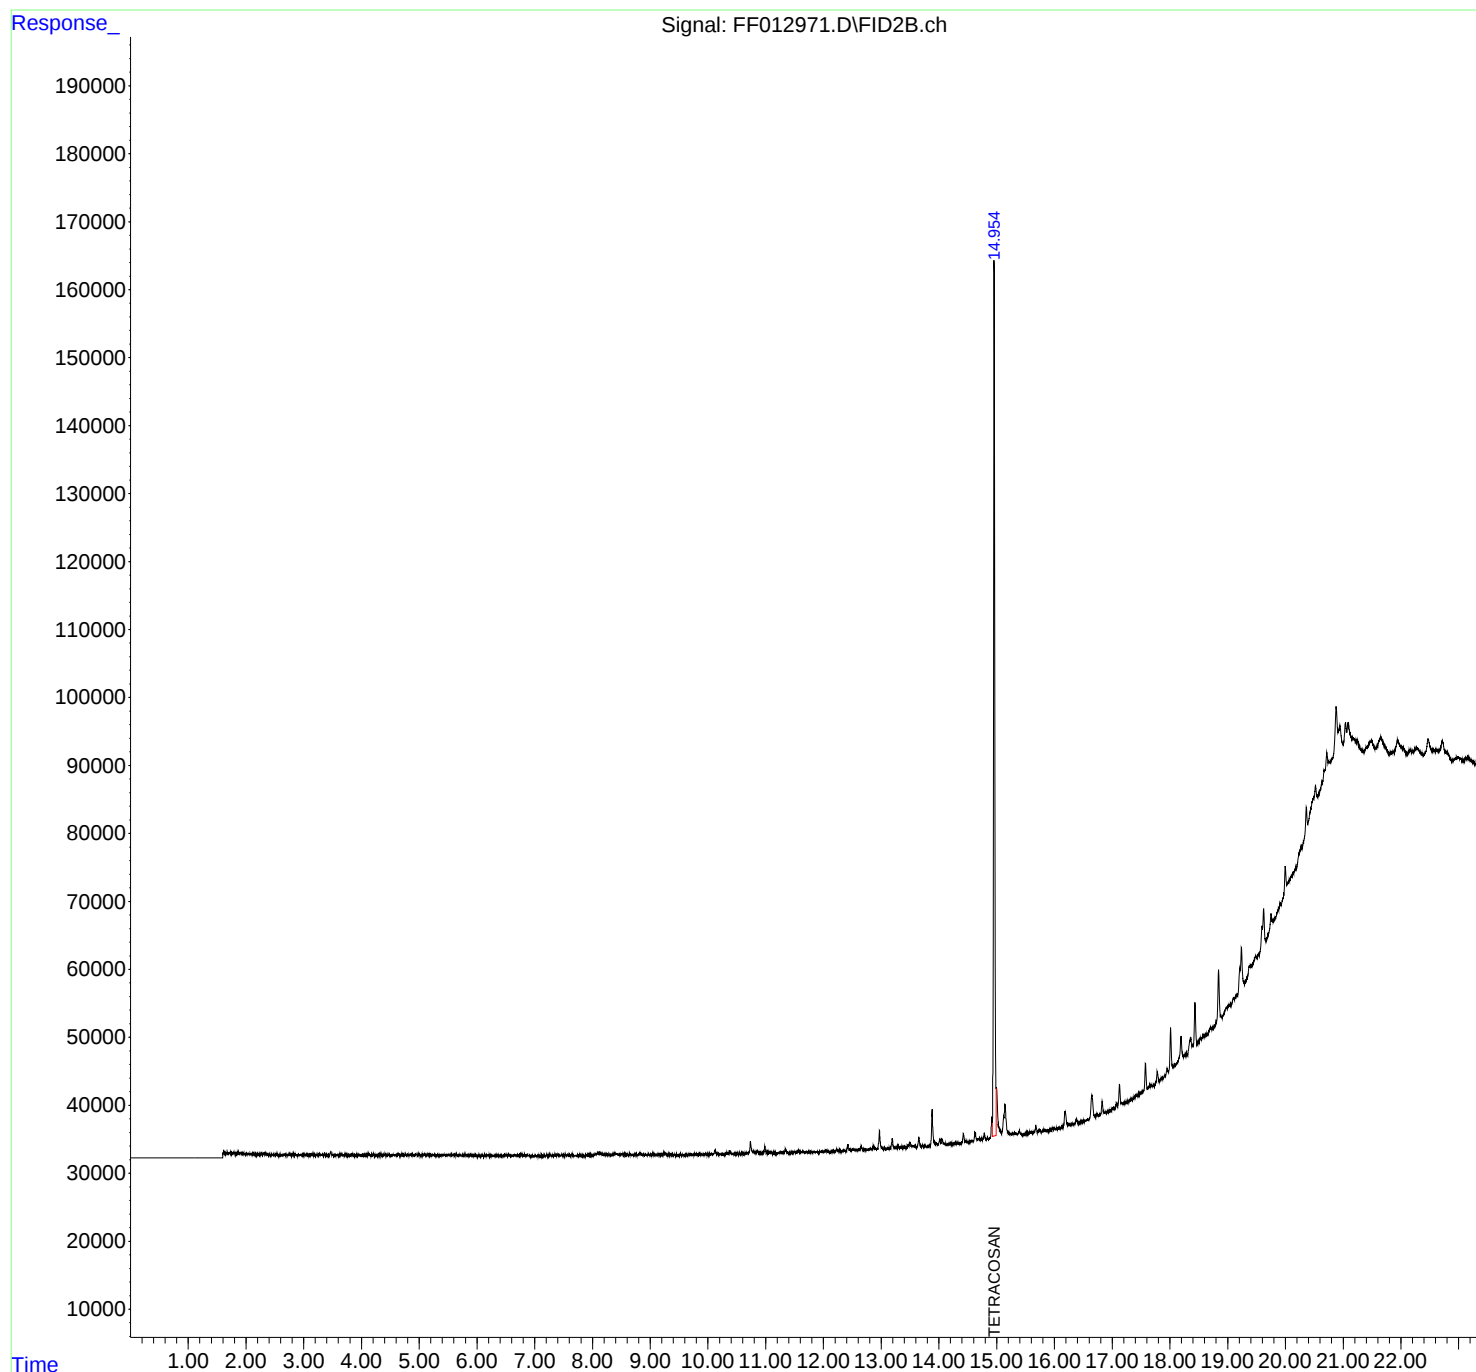

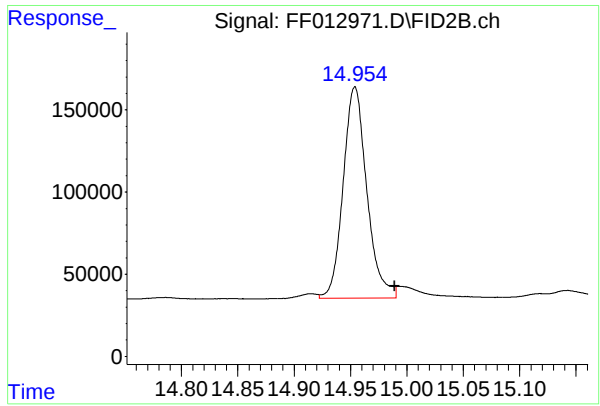

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.954 min  
Delta R.T.: -0.035 min  
Response: 1879870  
Conc: 16.10 ug/ml

Instrument :

FID\_F

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/24/2023

Supervised By :Ankita Jodhani 06/26/2023