

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323AL\
 Data File : FF012973.D
 Signal(s) : FID2B.ch
 Acq On : 23 Jun 2023 14:46
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 23 16:17:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 13:45:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	n-Tetracosane (C24)	14.142	63361	0.516 ug/ml
17) T	n-Tricontane (C30)	17.015	20787	0.175 ug/ml
18) T	n-Dotriacontane (C32)	17.842	160406	1.372 ug/ml
19) T	n-Tetratriacontane (C34)	18.626	17285	0.156 ug/ml
20) T	n-Hexatriacontane (C36)	19.366	125562	1.184 ug/ml
21) T	n-Octatriacontane (C38)	20.085	42110	0.403 ug/ml
22) T	n-Tetracontane (C40)	20.959	59274	0.612 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF062323AL\
Data File : FF012973.D
Signal(s) : FID2B.ch
Acq On : 23 Jun 2023 14:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 16:17:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 13:45:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

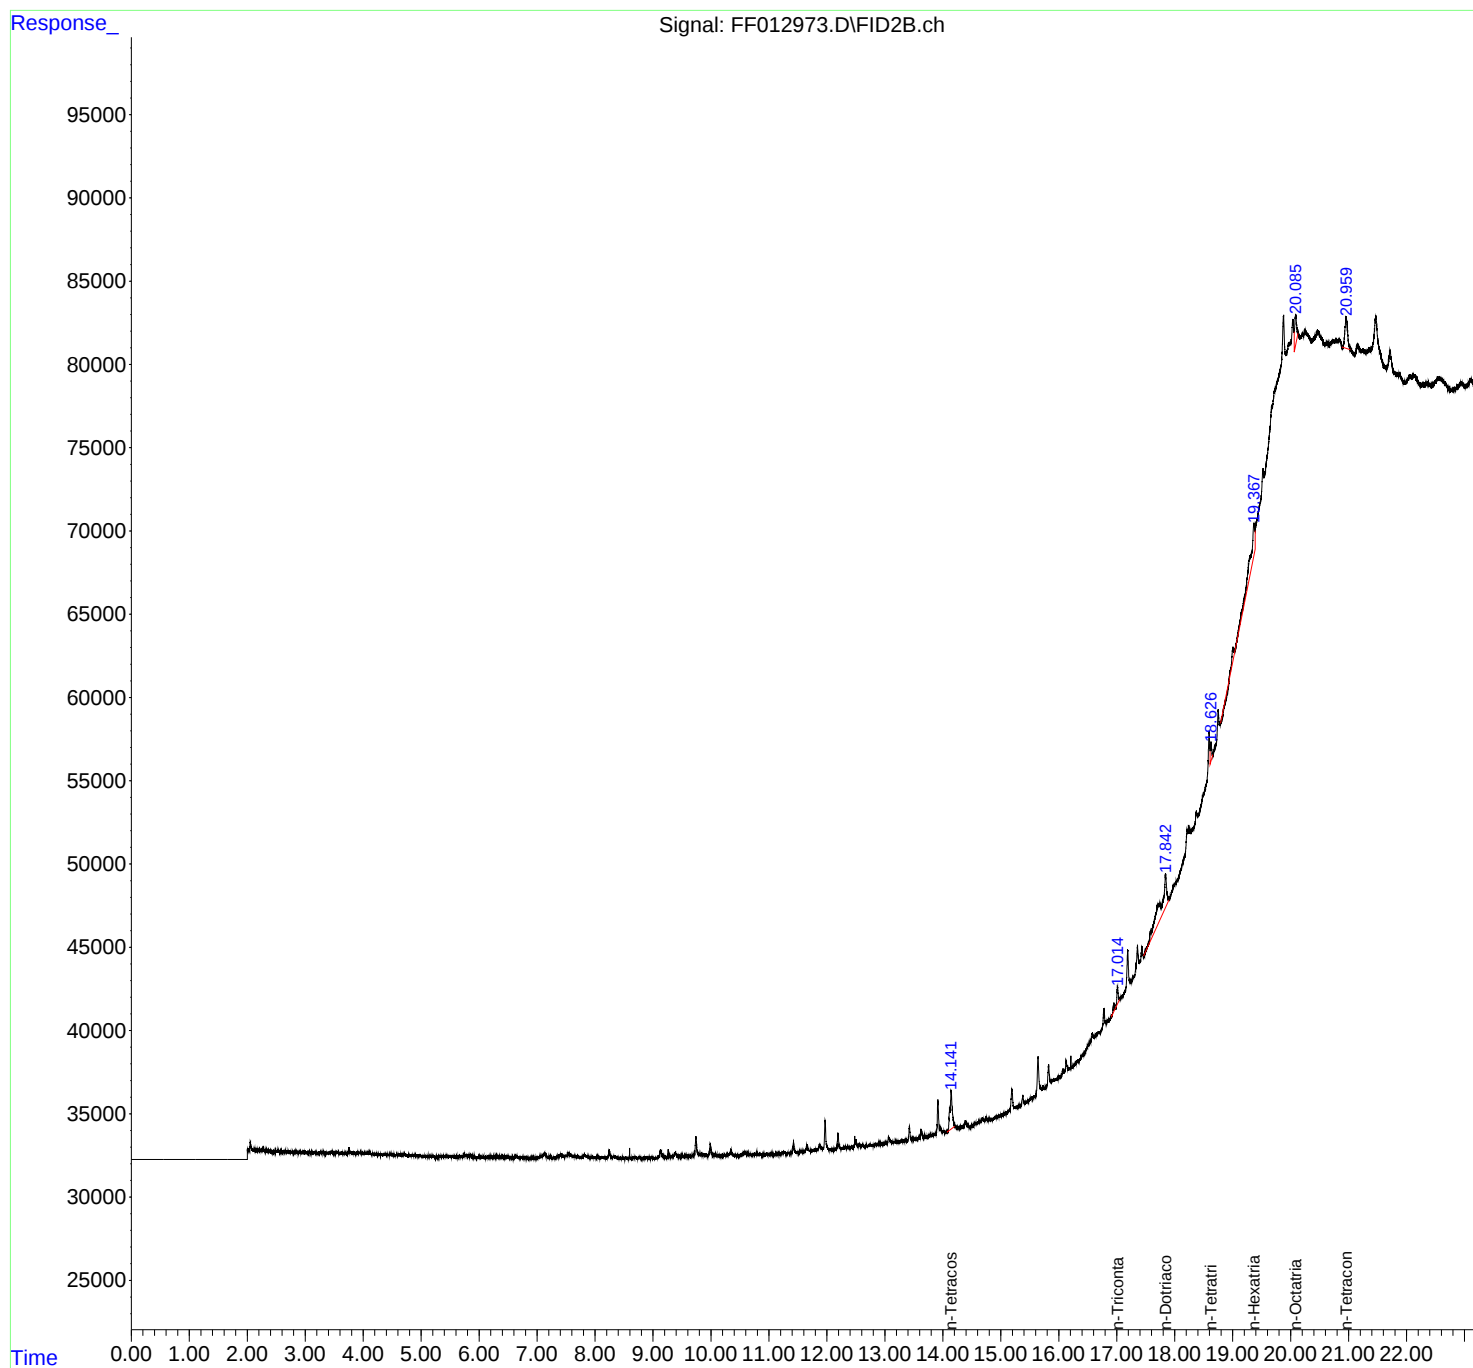


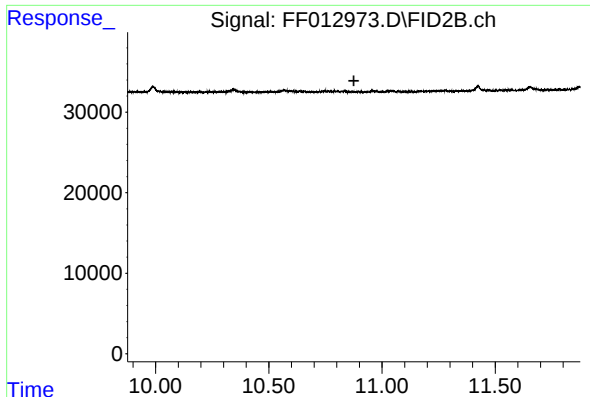

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.876 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

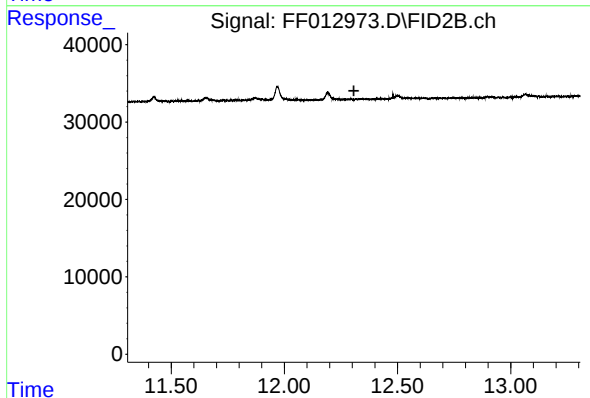


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.307 min
Response: 0
Conc: N.D.

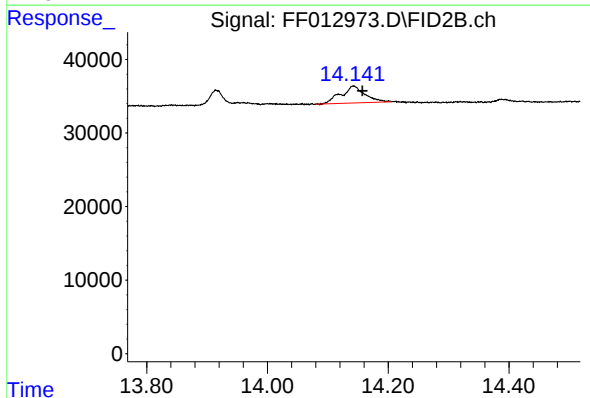


#14 n-Tetracosane (C24)

R.T.: 14.142 min
Delta R.T.: -0.015 min
Response: 63361
Conc: 0.52 ug/ml

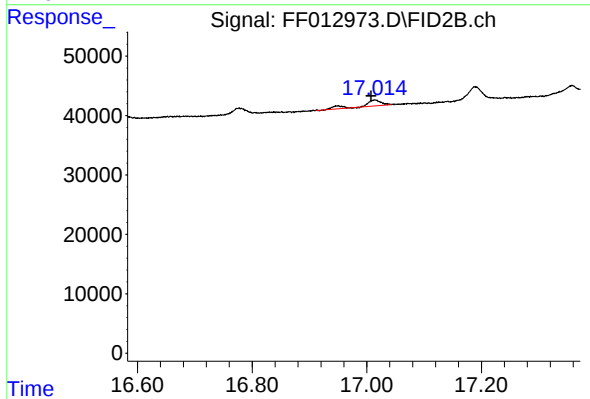

#17 n-Tricontane (C30)


R.T.: 17.015 min
Delta R.T.: 0.007 min
Response: 20787
Conc: 0.17 ug/ml

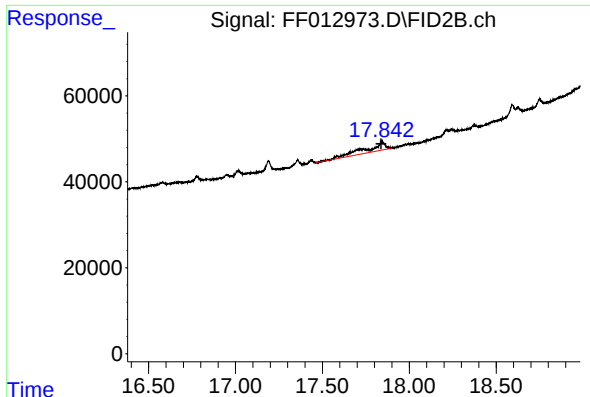

#18 n-Dotriacontane (C32)


R.T.: 17.842 min
Delta R.T.: 0.005 min
Response: 160406
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :

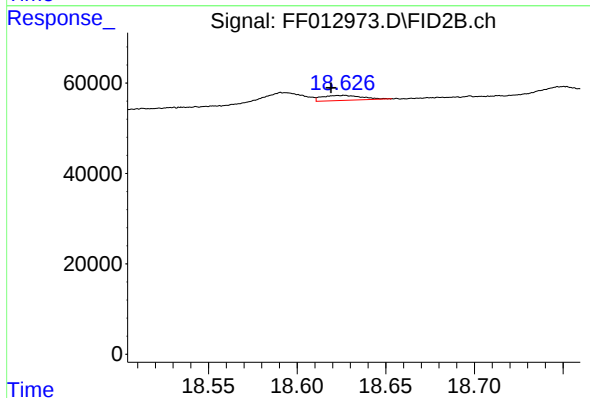


#19 n-Tetratriacontane (C34)

R.T.: 18.626 min
Delta R.T.: 0.007 min
Response: 17285
Conc: 0.16 ug/ml

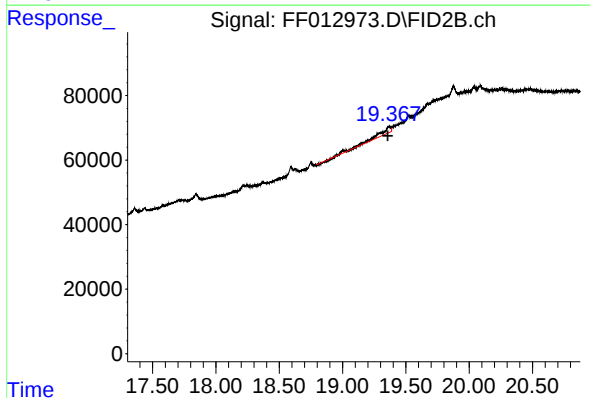


#20 n-Hexatriacontane (C36)

R.T.: 19.366 min
Delta R.T.: 0.009 min
Response: 125562
Conc: 1.18 ug/ml

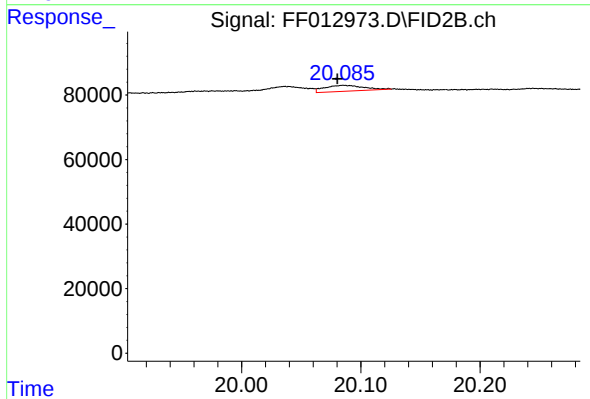

#21 n-Octatriacontane (C38)

R.T.: 20.085 min
Delta R.T.: 0.005 min
Response: 42110
Conc: 0.40 ug/ml

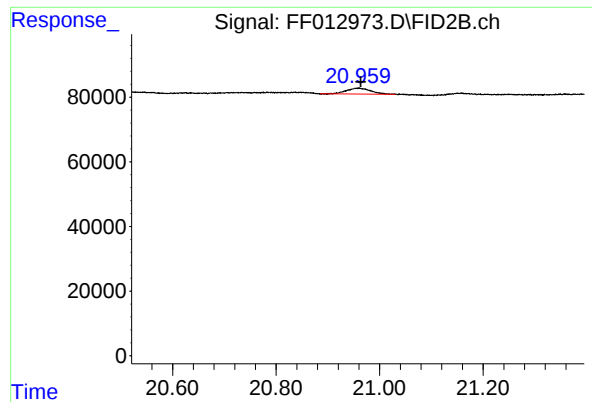

#22 n-Tetracontane (C40)

R.T.: 20.959 min
Delta R.T.: -0.004 min
Response: 59274
Conc: 0.61 ug/ml

Instrument :

FID_F

ClientSampleId :